




Pile Dynamics, Inc.

Transducer 8131

Strain ($\mu\epsilon$)

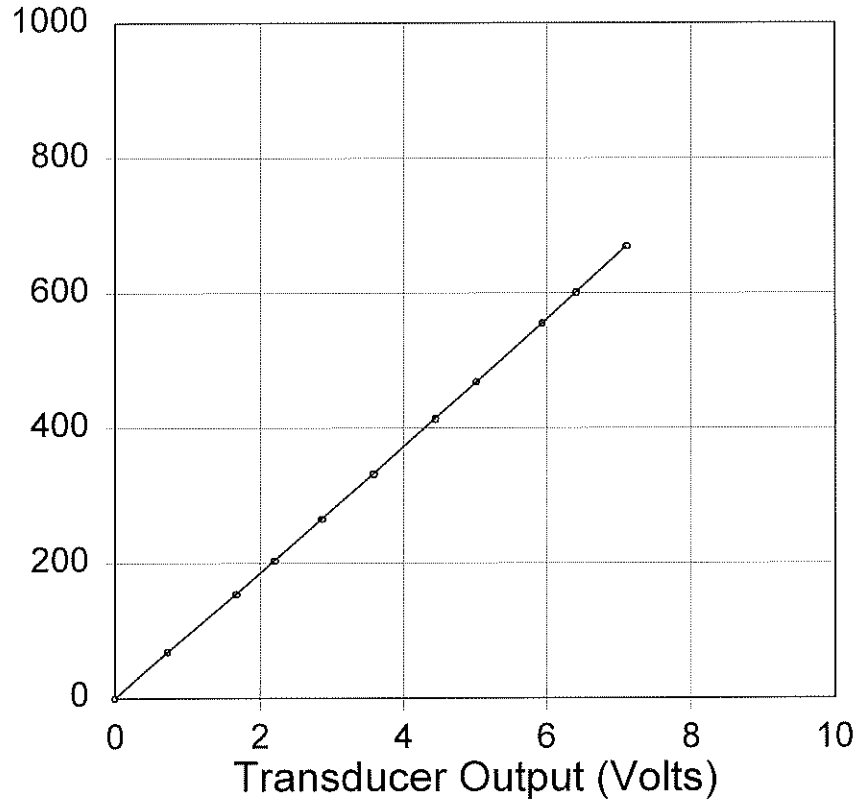

PDA Cal Factor 94.0 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
68	0.72
153	1.65
203	2.19
264	2.85
331	3.57
414	4.44
468	5.01
556	5.94
601	6.40
669	7.11

Shunt (60.4 K Ω) 5.0 V
 General Factor 326.3 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by: *R. Eason*
 Calibrated on: 04-Feb-2004