




# Pile Dynamics, Inc.

## Transducer 8132

Strain ( $\mu\epsilon$ )

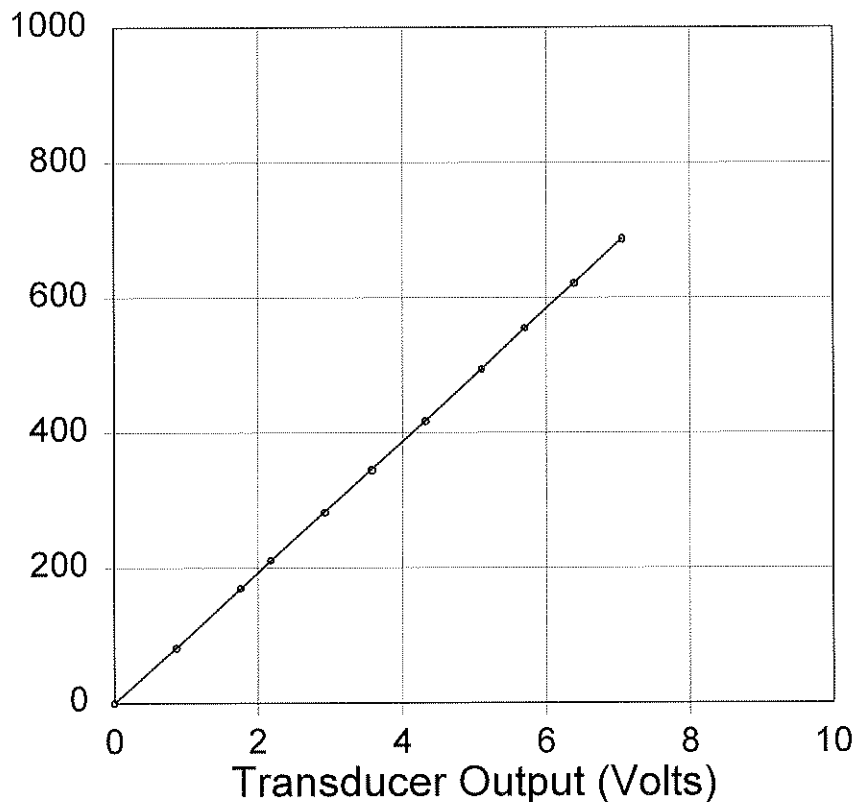

PDA Cal Factor

97.6 $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
82	0.86
170	1.77
210	2.18
282	2.92
345	3.57
417	4.31
494	5.10
554	5.70
622	6.39
687	7.05

Shunt (60.4 K $\Omega$ )

5.0 V

General Factor

338.9 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by:

Calibrated on:

25-Feb-2004