


Pile Dynamics Inc Transducer 4027

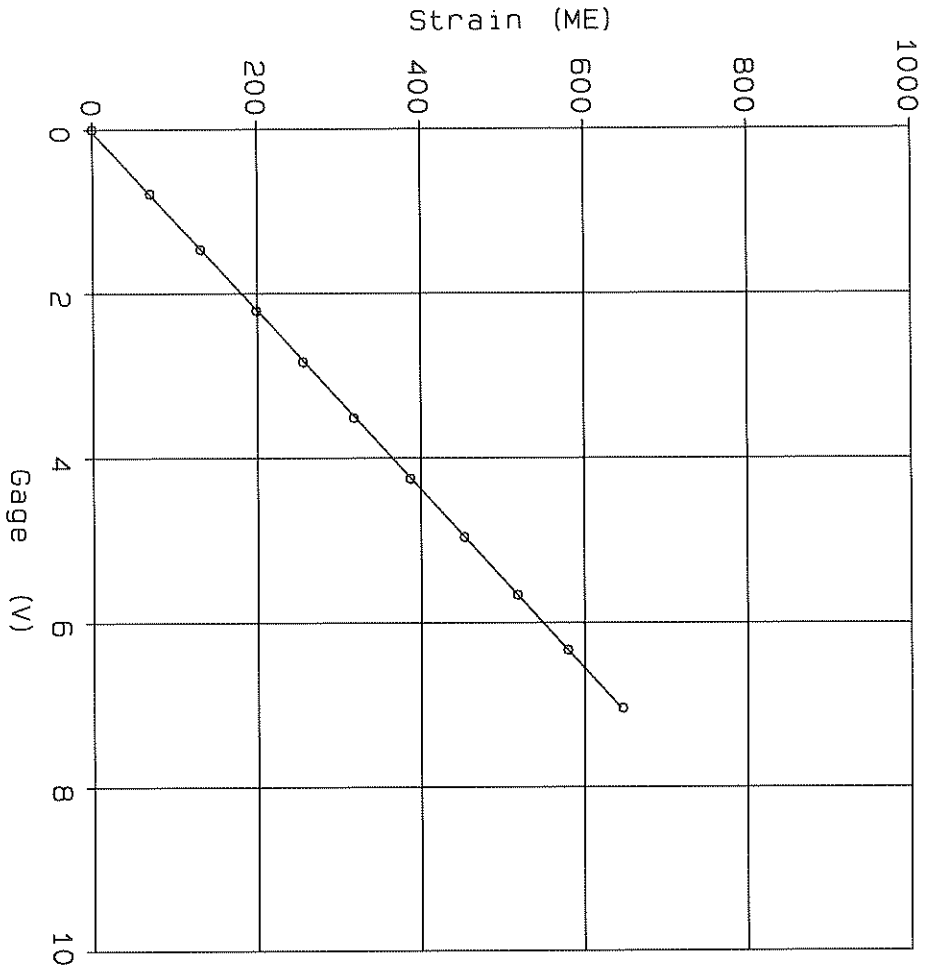

PDA Cal Factor = 92.0 ME/V
 Shunt (60.4K Ω) = 5.0 V
 General Factor = 319.3 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
70	.79
132	1.47
199	2.21
256	2.84
319	3.51
387	4.25
453	4.97
519	5.67
581	6.34
648	7.05

Calibrated by: B. S. [Signature]
 Calibrated on: 28-Dec-98