


# Pile Dynamics Inc Transducer 4028

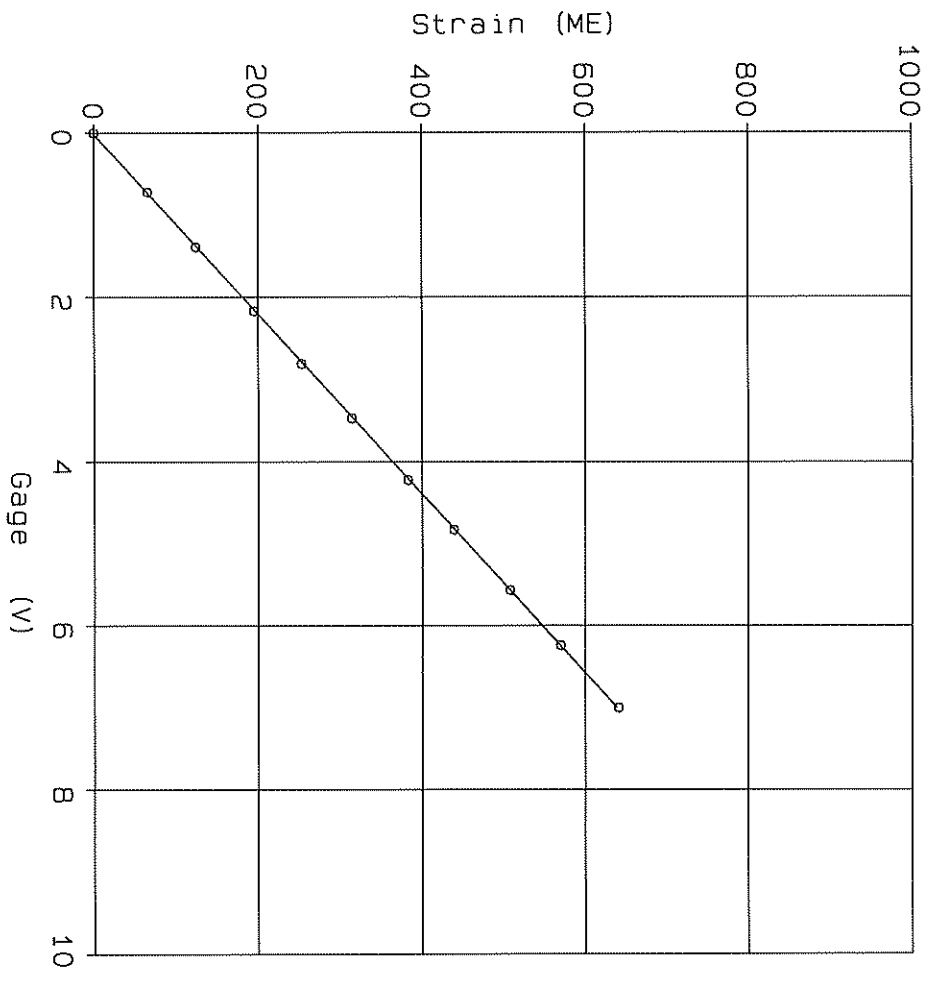

PDA Cal Factor = 91.6 ME/V  
 Shunt (60.4K0) = 5.0 V  
 General Factor = 318.0 ME/mv/V  
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
65	.73
125	1.39
196	2.17
253	2.81
315	3.48
383	4.23
440	4.83
508	5.58
571	6.25
642	7.01

Calibrated by: *B. Sauer*  
 Calibrated on: ~~28-Dec-98~~