


# Pile Dynamics Inc Transducer 4031

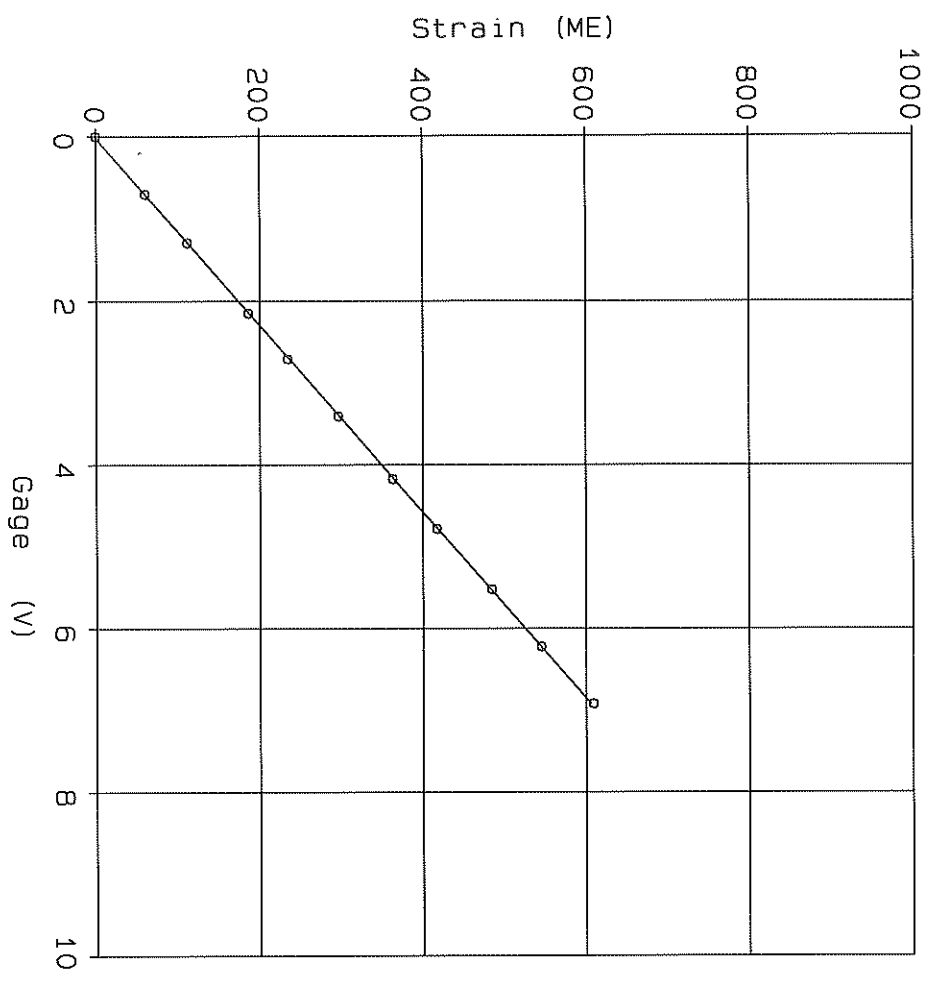

PDA Cal Factor = 88.0 ME/V  
 Shunt (60.4K0) = 5.0 V  
 General Factor = 305.7 ME/mv/V  
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
60	.70
112	1.30
186	2.16
235	2.71
297	3.41
364	4.18
418	4.78
484	5.53
546	6.22
609	6.92

Calibrated by: *B. Spoor*  
 Calibrated on: 12-Feb-99