




Pile Dynamics, Inc.

Transducer 4034

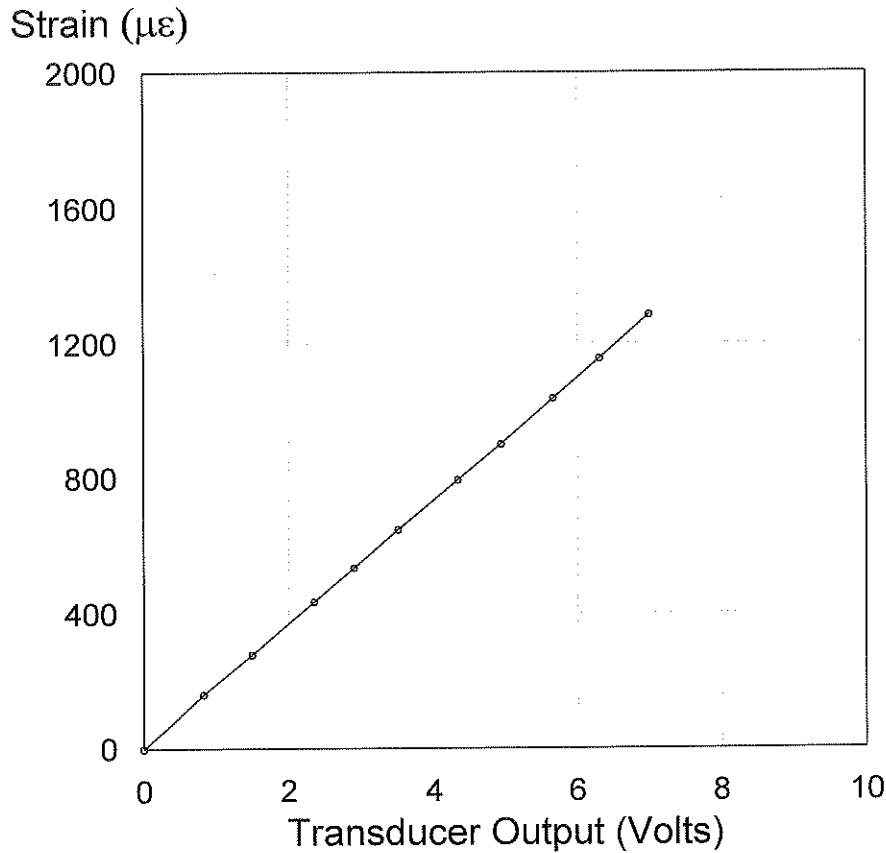


PDA Cal Factor (5.0 V) 91.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
161	0.82
278	1.49
433	2.35
533	2.91
646	3.51
794	4.33
900	4.93
1035	5.66
1155	6.31
1284	7.00

Shunt (60.4 K Ω) 2.5 V
 General Factor 316.3 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by: 
 Calibrated on: 16-Apr-2012