


Pile Dynamics Inc Transducer 4035

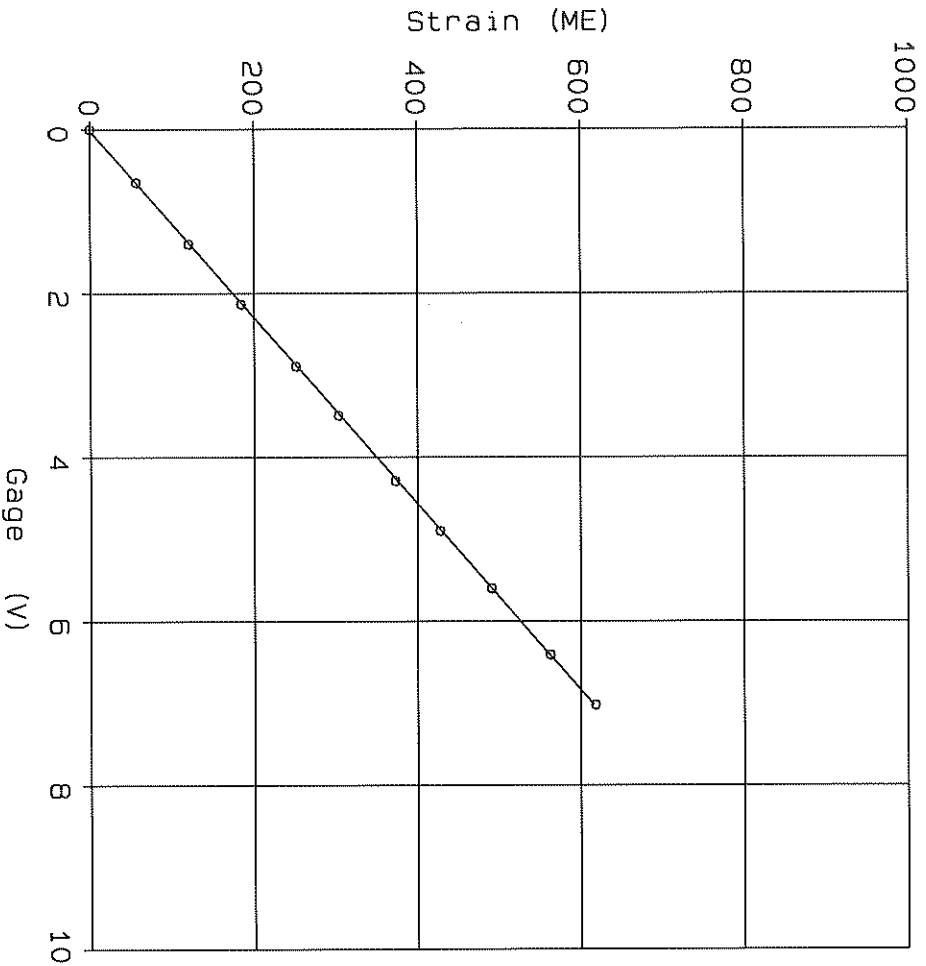

PDA Cal Factor = 88.0 ME/V
 Shunt (60.4K Ω) = 5.0 V
 General Factor = 305.7 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
56	.66
121	1.40
185	2.13
251	2.89
304	3.49
374	4.29
428	4.90
491	5.61
564	6.42
619	7.03

Calibrated by: B. Swann
 Calibrated on: 12-Feb-99