


Pile Dynamics Inc Transducer 4036

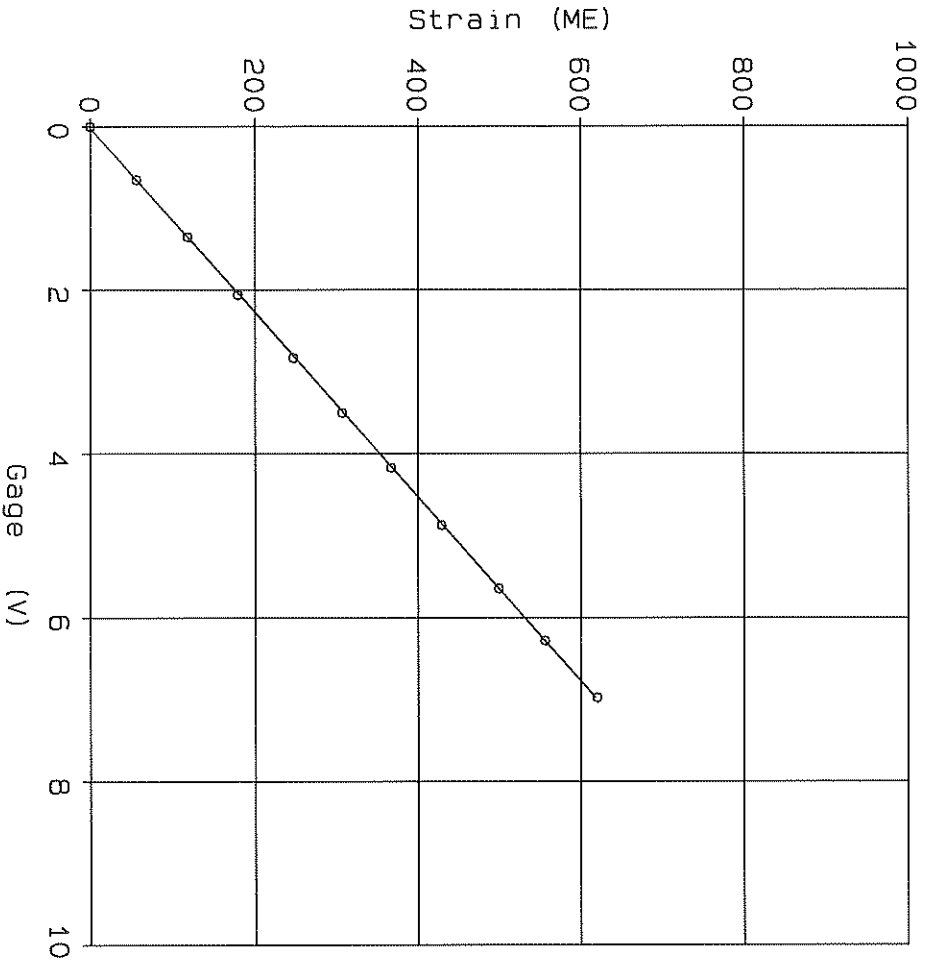

PDA Cal Factor = 88.8 ME/V
 Shunt (60.4K0) = 5.0 V
 General Factor = 308.4 ME/mv/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
57	.66
118	1.36
180	2.07
248	2.83
308	3.51
367	4.18
430	4.88
499	5.65
557	6.28
620	6.99

Calibrated by: B. Swann
 Calibrated on: 11-Feb-99