


Pile Dynamics Inc Transducer 4037

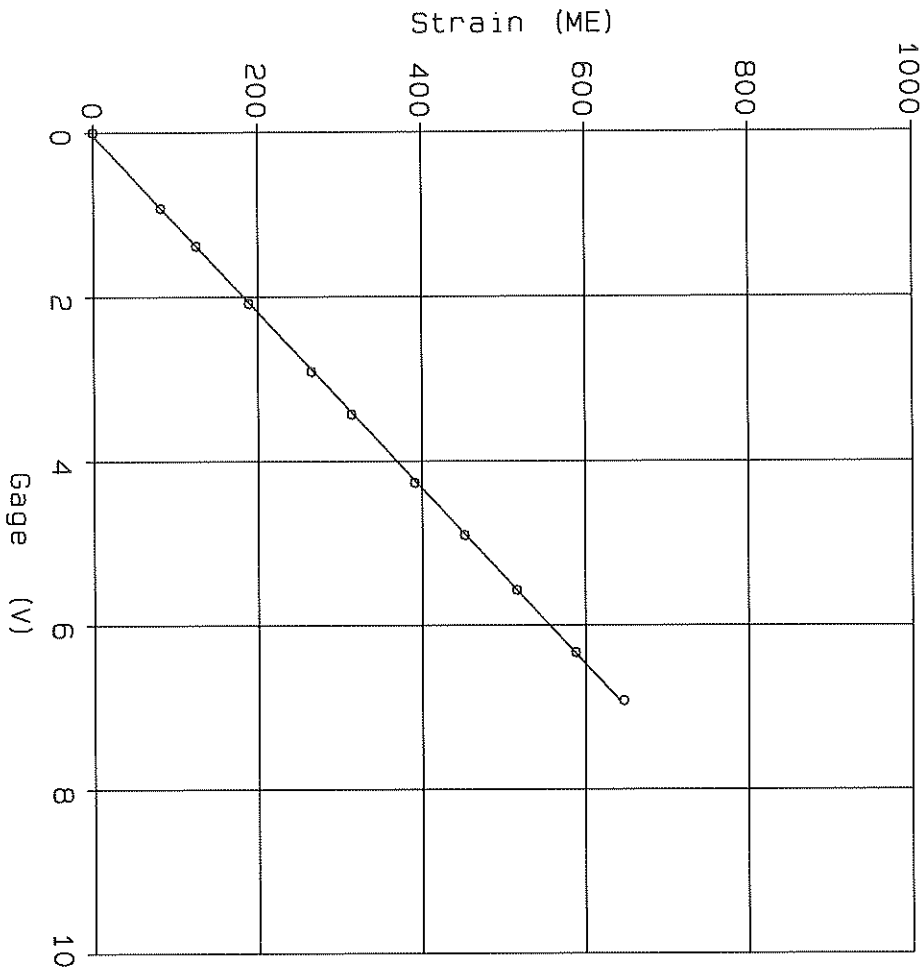

PDA Cal Factor = 93.4 ME/V
 Shunt (60.4K Ω) = 5.0 V
 General Factor = 324.2 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
83	.92
125	1.39
189	2.09
266	2.92
314	3.43
391	4.26
452	4.91
516	5.57
588	6.34
647	6.93

Calibrated by: B. Sauer
 Calibrated on: 27-Apr-99