


Pile Dynamics Inc Transducer 4038

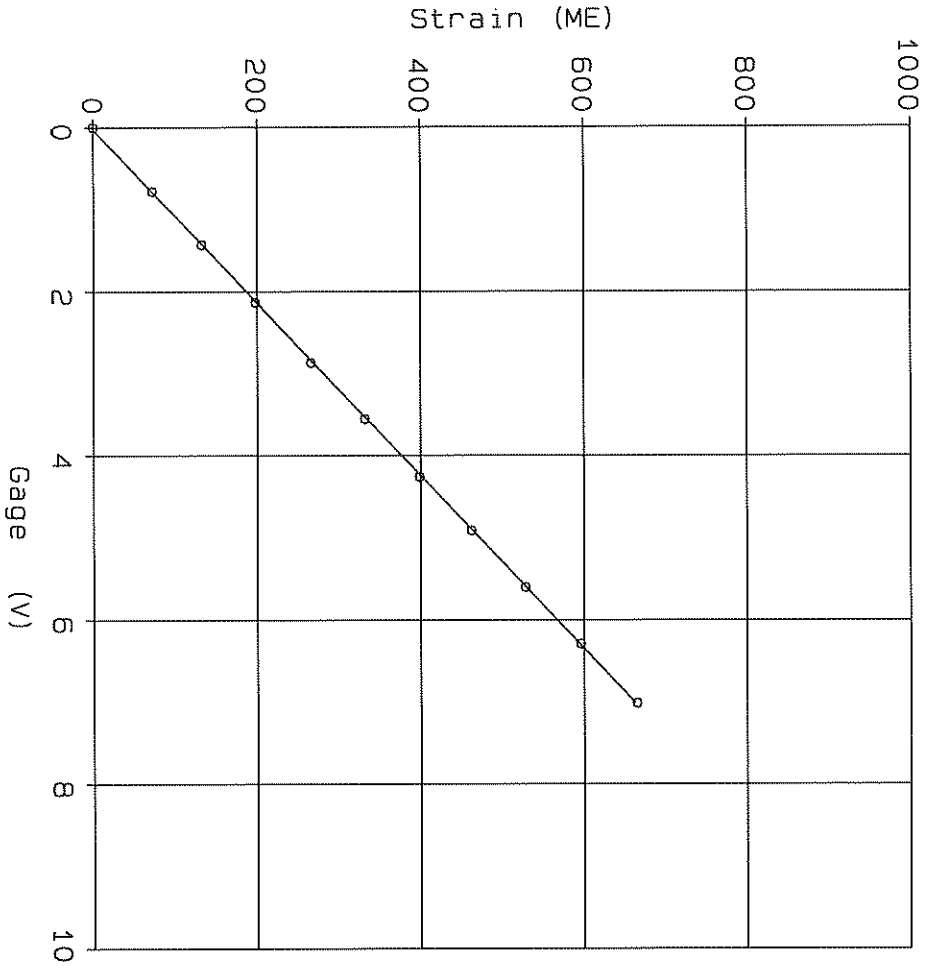

PDA Cal Factor = 95.0 ME/V
 Shunt (60.4K Ω) = 5.0 V
 General Factor = 329.8 ME/mv/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
72	.79
132	1.43
198	2.14
266	2.86
332	3.55
400	4.26
462	4.91
529	5.60
596	6.30
666	7.02

Calibrated by: *B. Savon*
 Calibrated on: 11-Feb-99