




Pile Dynamics, Inc.

Transducer 8953

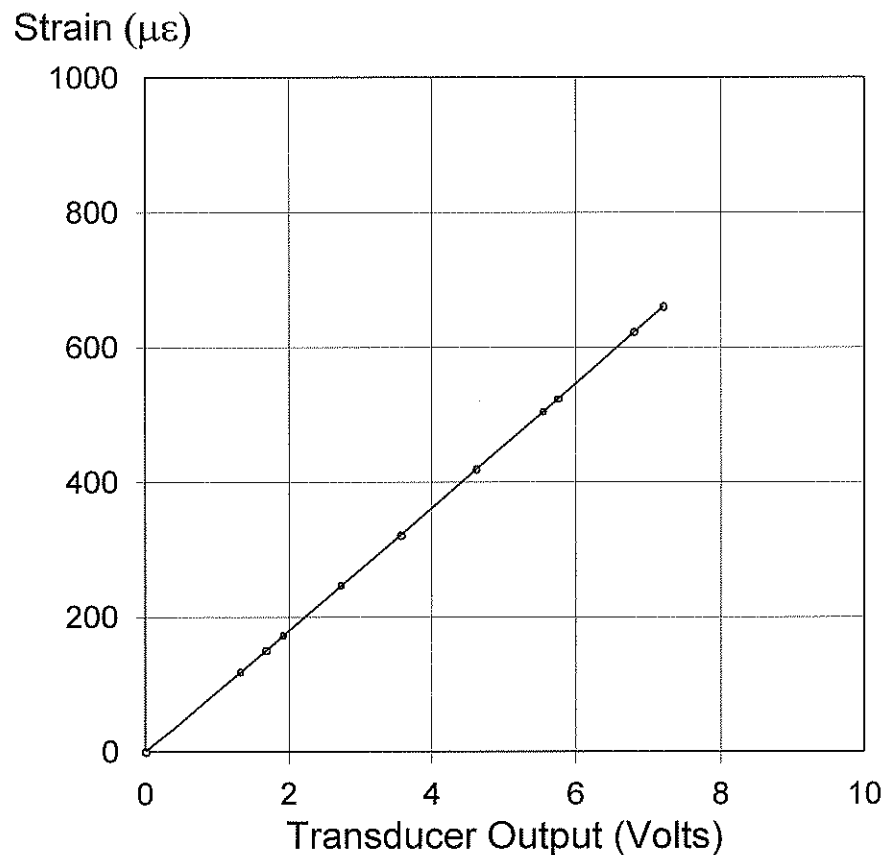

PDA Cal Factor 91.8 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
118	1.32
150	1.67
172	1.92
246	2.73
321	3.56
420	4.63
505	5.54
524	5.75
623	6.80
661	7.20

Shunt (60.4 K Ω) 5.0 V
 General Factor 318.9 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by:

Calibrated on:

R. Eason
 07-Jun-2005