




Pile Dynamics, Inc.

Transducer 8955

Strain ($\mu\epsilon$)

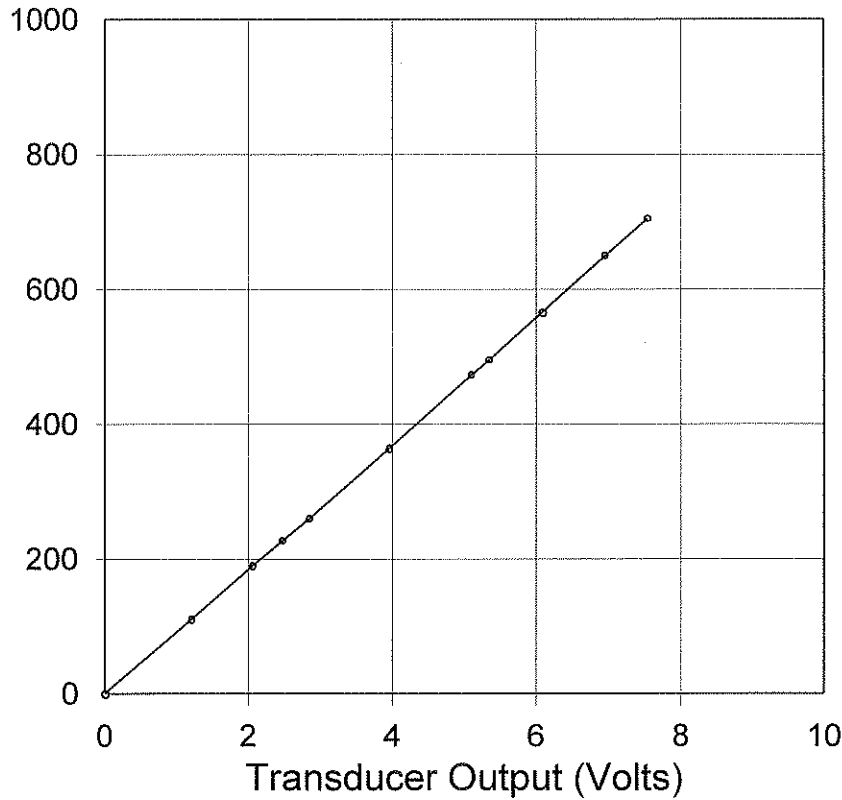

PDA Cal Factor

93.7 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
110	1.21
190	2.06
226	2.46
261	2.84
364	3.95
473	5.11
496	5.34
566	6.08
650	6.95
705	7.53

Shunt (60.4 K Ω)

5.0 V

General Factor

325.3 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by:

Calibrated on:

20-Apr-2005