




Pile Dynamics, Inc.

Transducer 8956

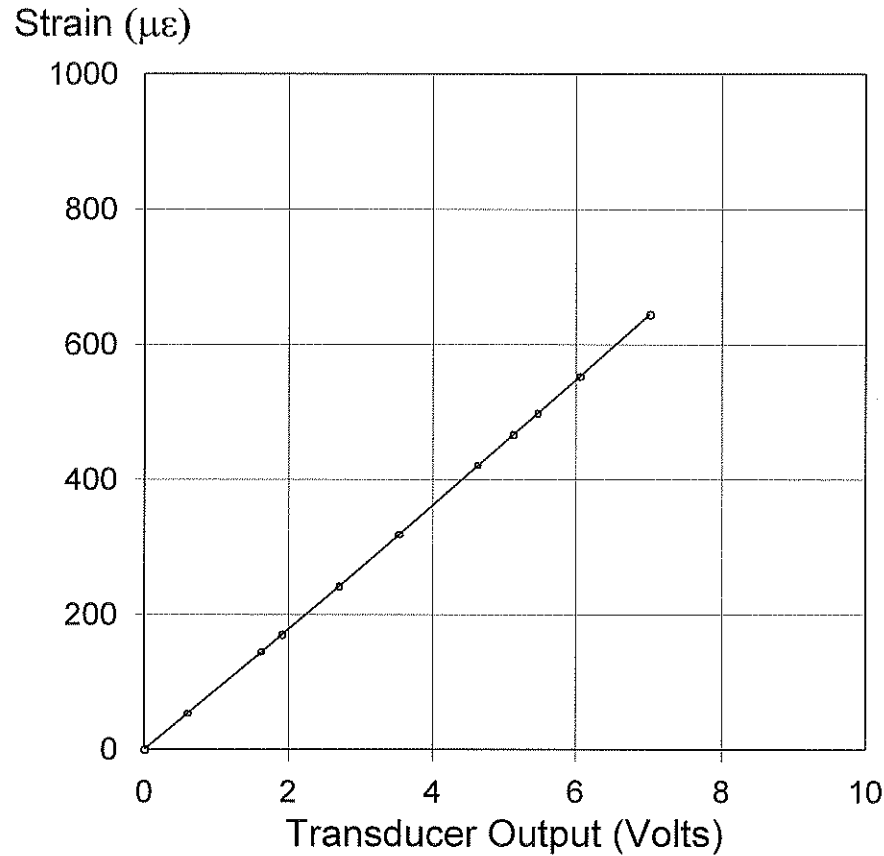

PDA Cal Factor 91.9 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
53	0.60
145	1.62
171	1.91
242	2.70
318	3.52
421	4.62
466	5.12
499	5.47
553	6.04
644	7.01

Shunt (60.4 K Ω) 5.0 V
 General Factor 319.0 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by:

Calibrated on:

R. Eason
 11-Jan-2005