




Pile Dynamics, Inc.

Transducer 8958

Strain ($\mu\epsilon$)

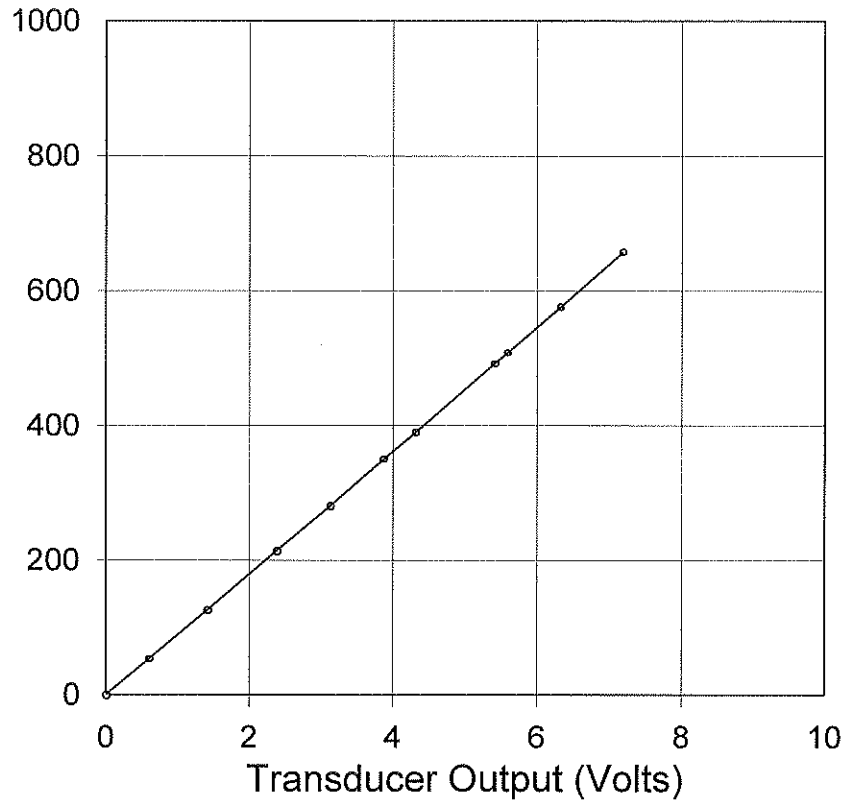

PDA Cal Factor

91.4 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
54	0.60
127	1.41
214	2.38
281	3.12
350	3.87
390	4.31
492	5.41
508	5.59
577	6.32
658	7.18

Shunt (60.4 K Ω)

5.0 V

General Factor

317.5 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

20-Apr-2005