


# Pile Dynamics, Inc.

## Transducer 8959

Strain ( $\mu\epsilon$ )

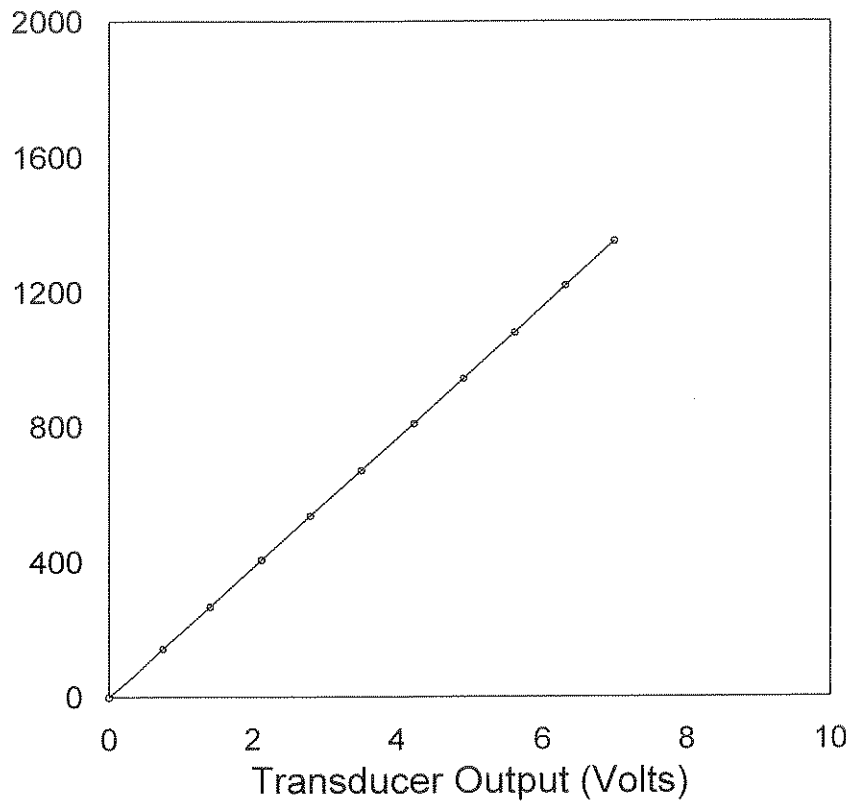

PDA Cal Factor (5.0 V)

96.5 $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
143	0.74
268	1.40
407	2.12
536	2.80
670	3.51
809	4.23
943	4.91
1079	5.61
1220	6.31
1352	6.99

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

335.2 $\mu\epsilon/mV/V$

Calibrated by:

*Greg Rasmussen*

Calibrated on:

26-May-2011

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Smart Sensor?  Yes  No Smart Chip Programmed by: GP on: 5/26/11 CRC value F90E