




Pile Dynamics, Inc.

Pile Dynamics, Inc.

Transducer

8964

Strain ($\mu\epsilon$)

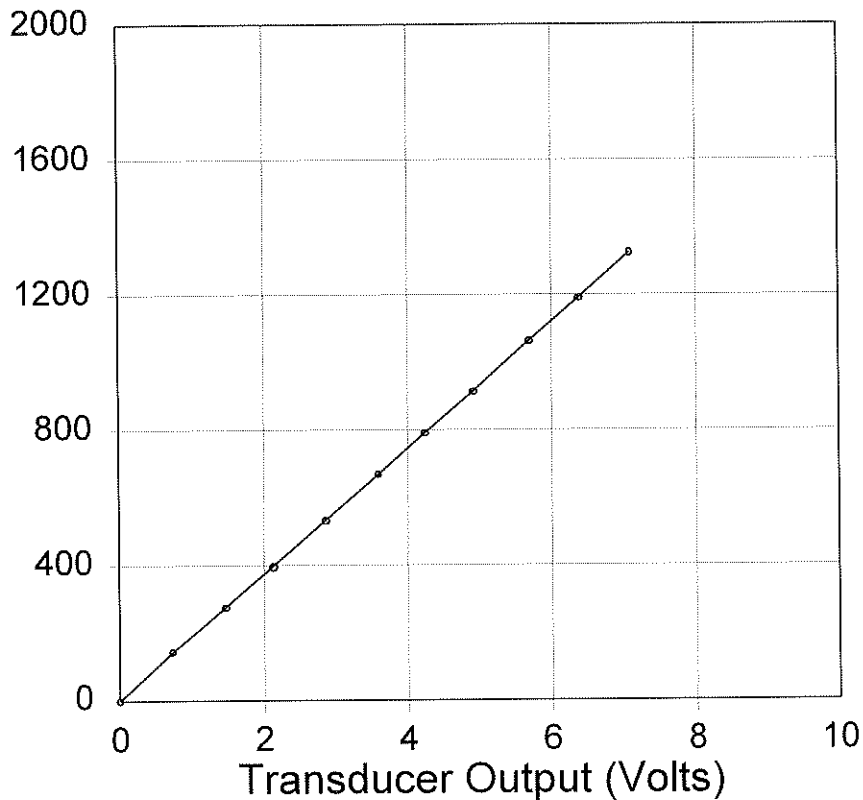

PDA Cal Factor (5.0 V) 93.3 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
145	0.73
273	1.46
395	2.12
532	2.85
668	3.59
789	4.23
913	4.91
1065	5.69
1189	6.37
1326	7.08

Shunt (60.4 K Ω)

2.5 V

General Factor

323.8 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

05-Feb-2007