




Pile Dynamics, Inc.

Transducer 9037

Strain ($\mu\epsilon$)

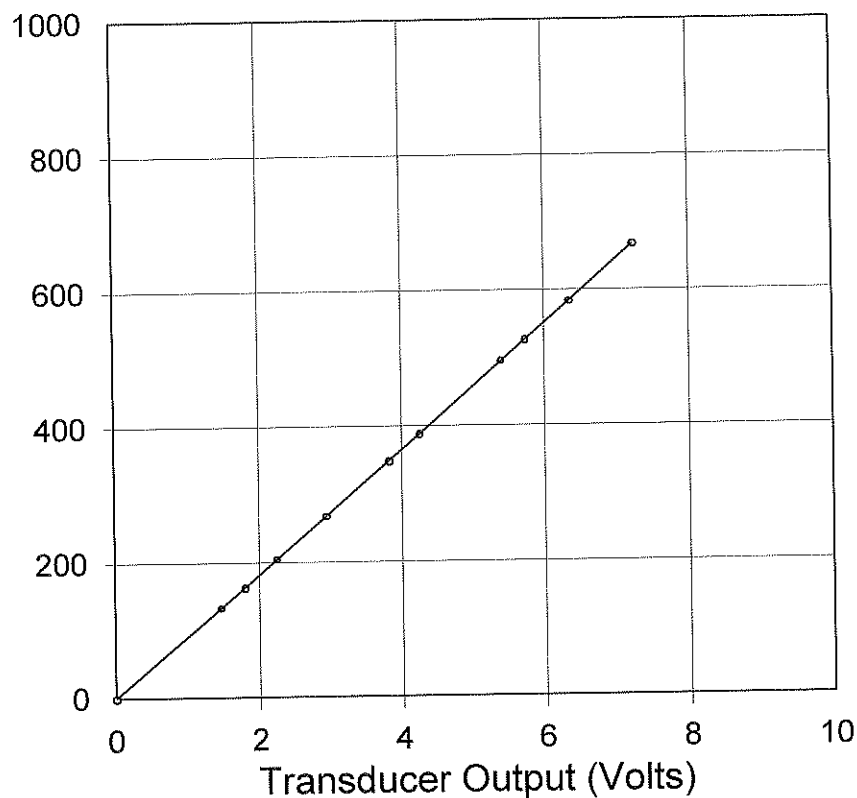

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

PDA Cal Factor

92.3 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
133	1.46
163	1.79
204	2.25
267	2.93
348	3.81
388	4.25
495	5.39
526	5.74
582	6.34
668	7.23

Shunt (60.4 K Ω)

5.0 V

General Factor

320.4 $\mu\epsilon$ /mV/V

Calibrated by:

Calibrated on:

B. Eason
27-Apr-2005