




Pile Dynamics, Inc.

Transducer 9048

Strain ($\mu\epsilon$)

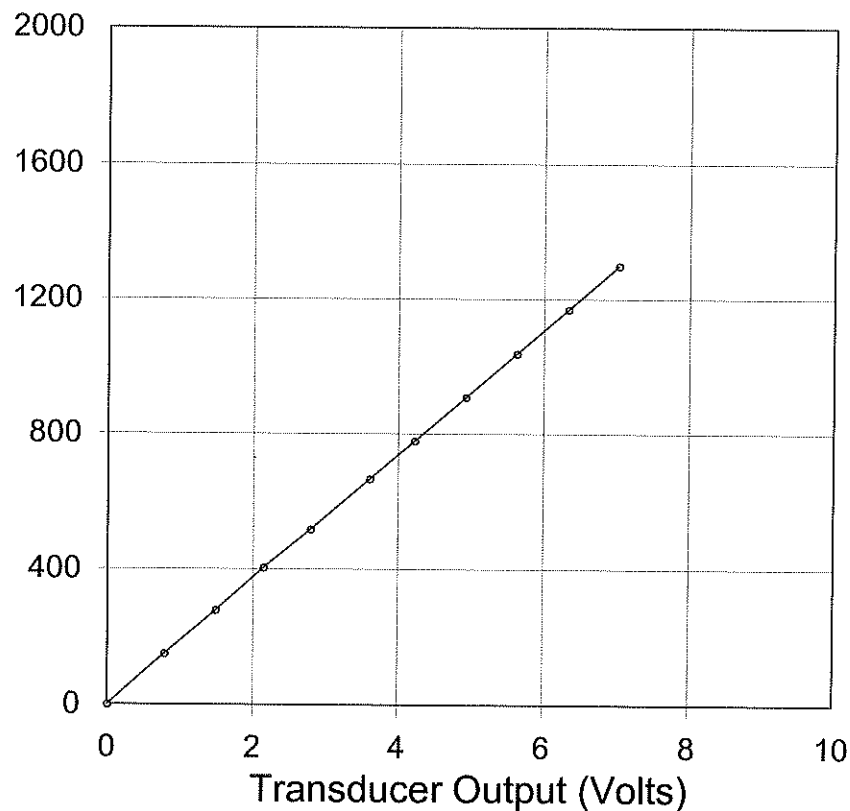

PDA Cal Factor (5.0 V)

92.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
151	0.78
279	1.48
404	2.14
516	2.79
665	3.60
779	4.22
907	4.92
1037	5.62
1170	6.33
1300	7.02

Shunt (60.4 K Ω)

2.5 V

General Factor

319.8 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by:

Calibrated on:

15-Jan-2010