


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

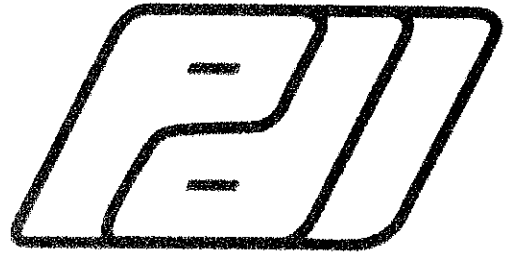

Serial No: K5729 Temperature: 23.1 °C
 Model: KICHER PR Humidity: 31%
 Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR
353.3 mv/5000g
 (70.7 μ v/g)
 R²: 0.999970 [Chip programmed]

Ref Acc 1: 78270! Cal on: 11Jan2024
 971 g's/volt
 Ref Acc 2: 78268! Cal on: 11Jan2024
 986 g's/volt

Operator: William Johnson




Signed

Calibration valid 2 years

From: 07Nov2025

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

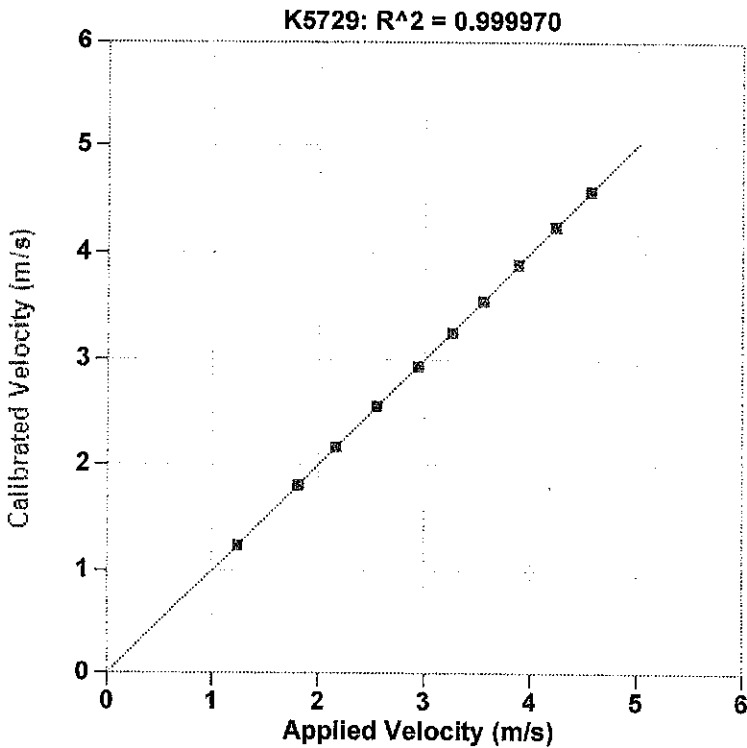

Reference Velocity	S/N K5729 Velocity
m/s	m/s
1.241	1.242
1.811	1.808
2.171	2.170
2.554	2.560
2.946	2.937
3.266	3.256
3.557	3.553
3.886	3.893
4.237	4.240
4.570	4.575

Maximum Acceleration: 998 g's