


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

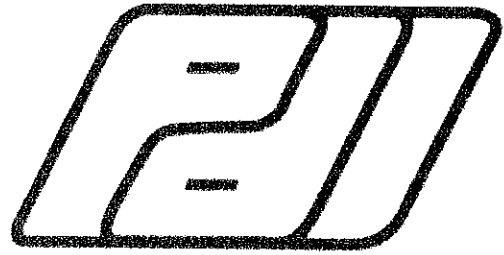

Serial No: K5730 Temperature: 23.1 °C
 Model: KICHER PR Humidity: 31%
 Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR
347.3 mv/5000g
 (69.5 μ v/g)
 R²: 0.999984 [Chip programmed]

Ref Acc 1: 78270! Cal on: 11Jan2024
 971 g's/volt
 Ref Acc 2: 78268! Cal on: 11Jan2024
 986 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 07Nov2025

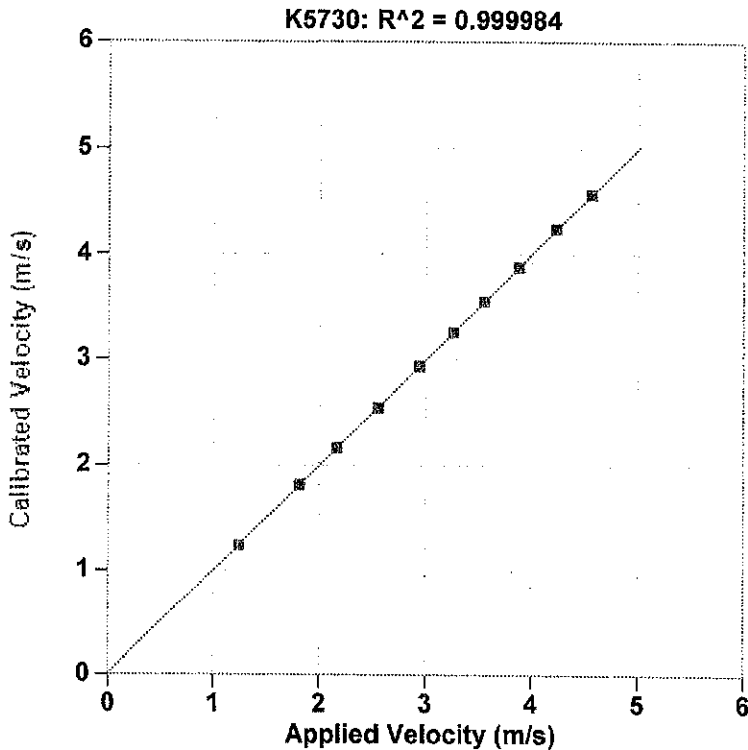

Reference Velocity	S/N K5730 Velocity
m/s	m/s
1.241	1.239
1.811	1.817
2.171	2.170
2.554	2.547
2.946	2.946
3.266	3.264
3.557	3.561
3.886	3.880
4.237	4.240
4.570	4.574

Maximum Acceleration: 998 g's