




# Certificate of Calibration

Pile Dynamics, Inc.  
 Transducer Model: PDI Strain Transducer  
 Serial Number: P042  
 PDI Gage Factor: 92.9  
 Mean Linear Correlation Coefficient: 0.999936

Table 1: Representative Calibration Data

Applied strain ( $\mu E$ )	Gage Output (mV/Vexc)	Applied strain ( $\mu E$ )	Gage Output (mV/Vexc)
-2034.1	-6.305	603.7	1.987
-1561.7	-4.799	931.8	2.996
-1207.3	-3.703	1253.3	3.987
-879.3	-2.670	1581.4	4.970
-492.1	-1.470	1916.0	5.971
-91.9	-0.215	2014.4	6.261
288.7	0.983		

Calibration Curve

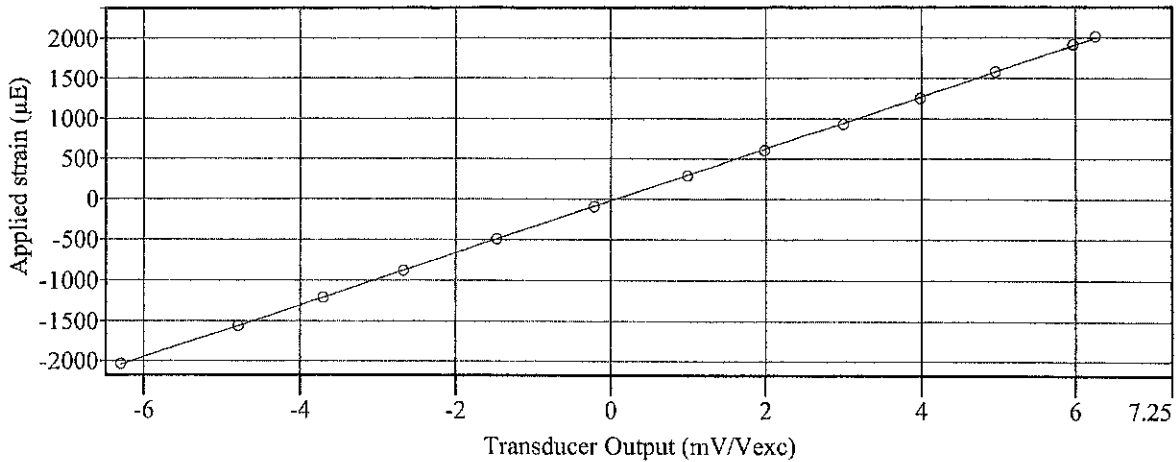

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: Paul Hartman

PDI Gage: P042

Calibration Date: 11/5/2025 6:52:50 AM

