


Pile Dynamics Inc Transducer 5110

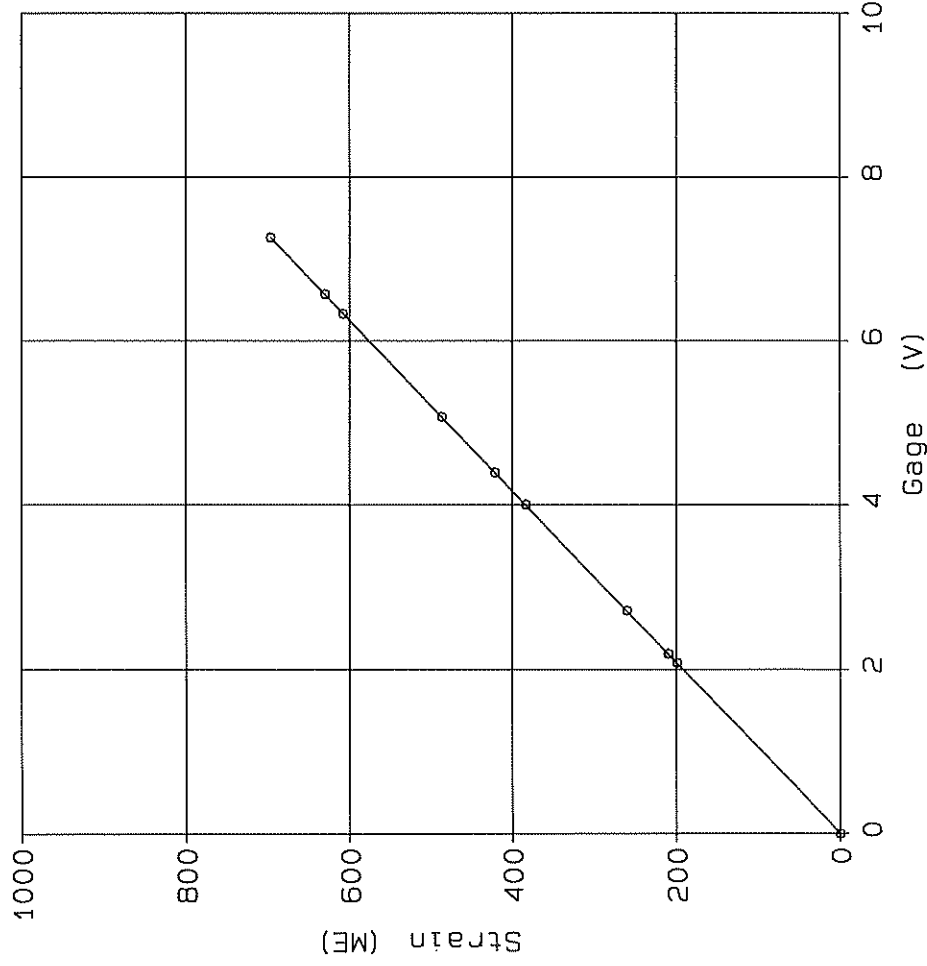

PDA Cal Factor = 96.0 ME/V
 Shunt (60.4K Ω) = 5.0 V
 General Factor = 333.5 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
200	2.09
210	2.20
210	2.19
261	2.73
384	4.00
421	4.40
487	5.07
608	6.33
630	6.57
697	7.27

Calibrated by: J. Denton
 Calibrated on: 29-Dec-00