


Pile Dynamics Inc Transducer 5111

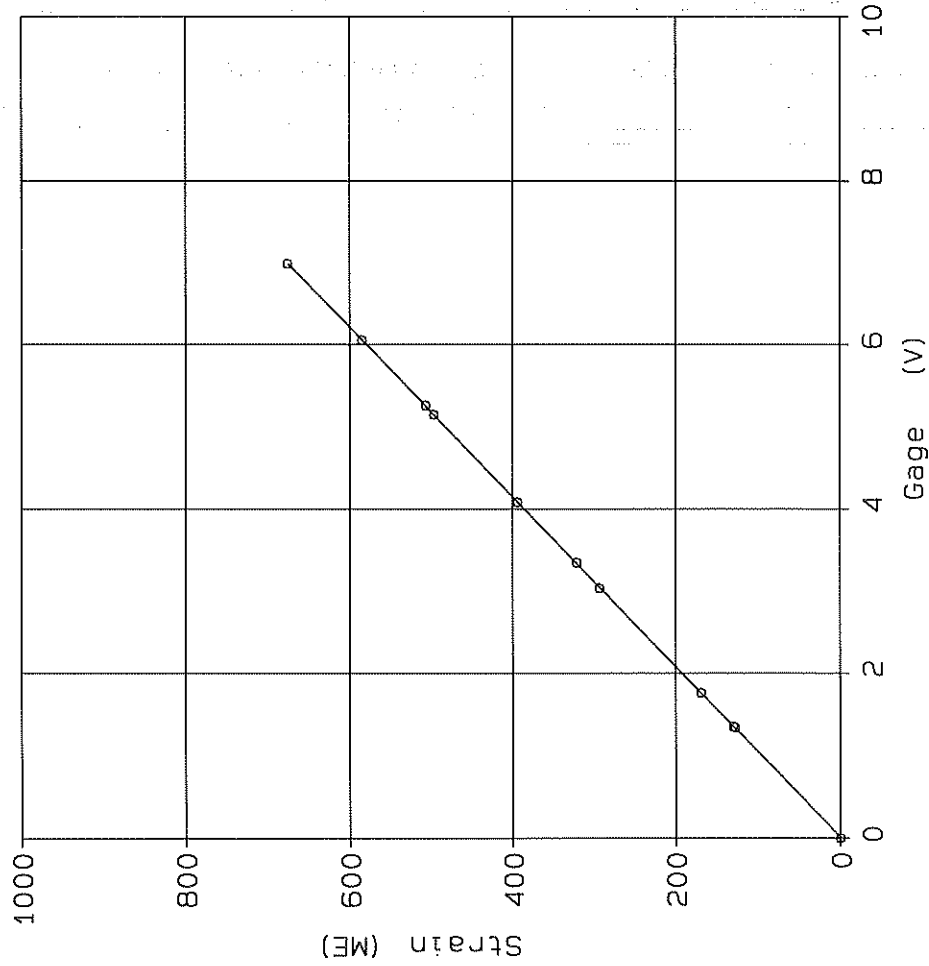

PDA Cal Factor = 96.8 ME/V
Shunt (60.4KΩ) = 5.0 V

General Factor = 336.0 ME/mV/V
Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
129	1.34
130	1.36
170	1.77
293	3.04
322	3.34
394	4.08
498	5.16
508	5.26
585	6.05
676	6.99

Calibrated by: J. Dentell

Calibrated on: 29-Dec-00