


Pile Dynamics Inc Transducer 5121

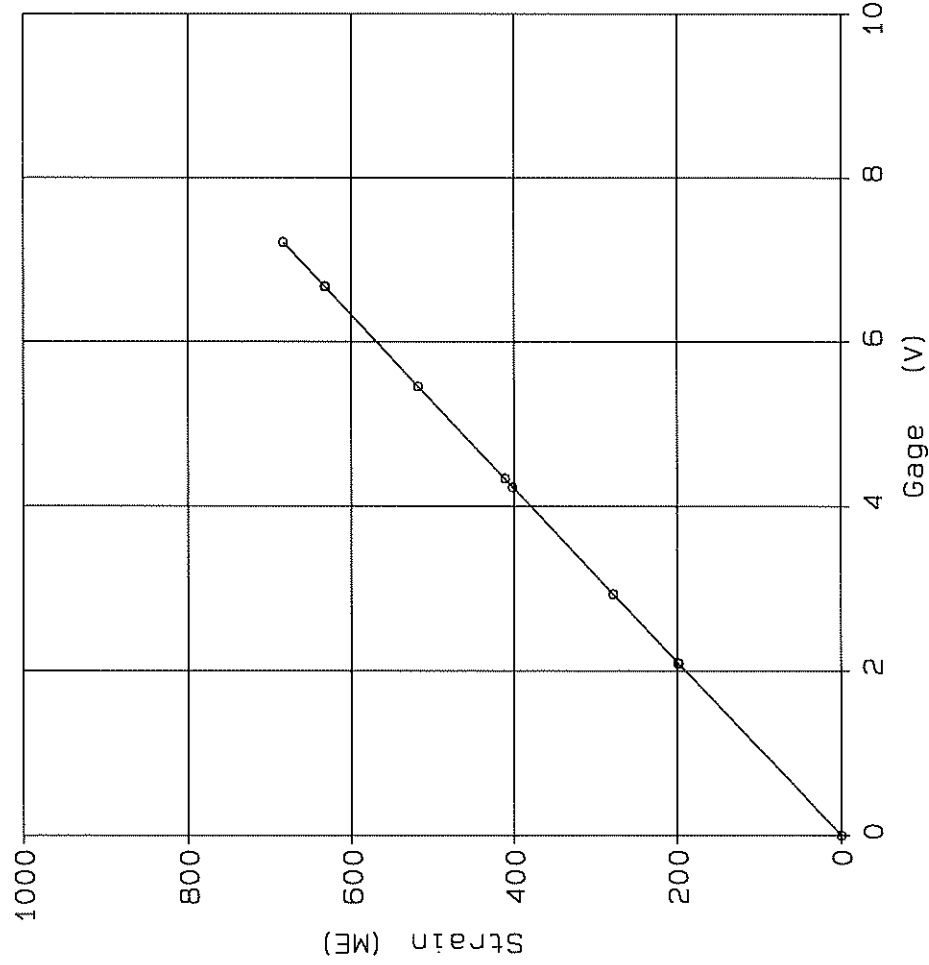

PDA Cal Factor = 95.0 ME/V
 Shunt (60.4K Ω) = 5.0 V
 General Factor = 329.9 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
199	2.11
198	2.10
200	2.11
279	2.94
402	4.24
412	4.35
519	5.46
634	6.67
633	6.67
685	7.21

Calibrated by: J. Dentel
 Calibrated on: 16-Jan-01