


Pile Dynamics Inc Transducer 5122

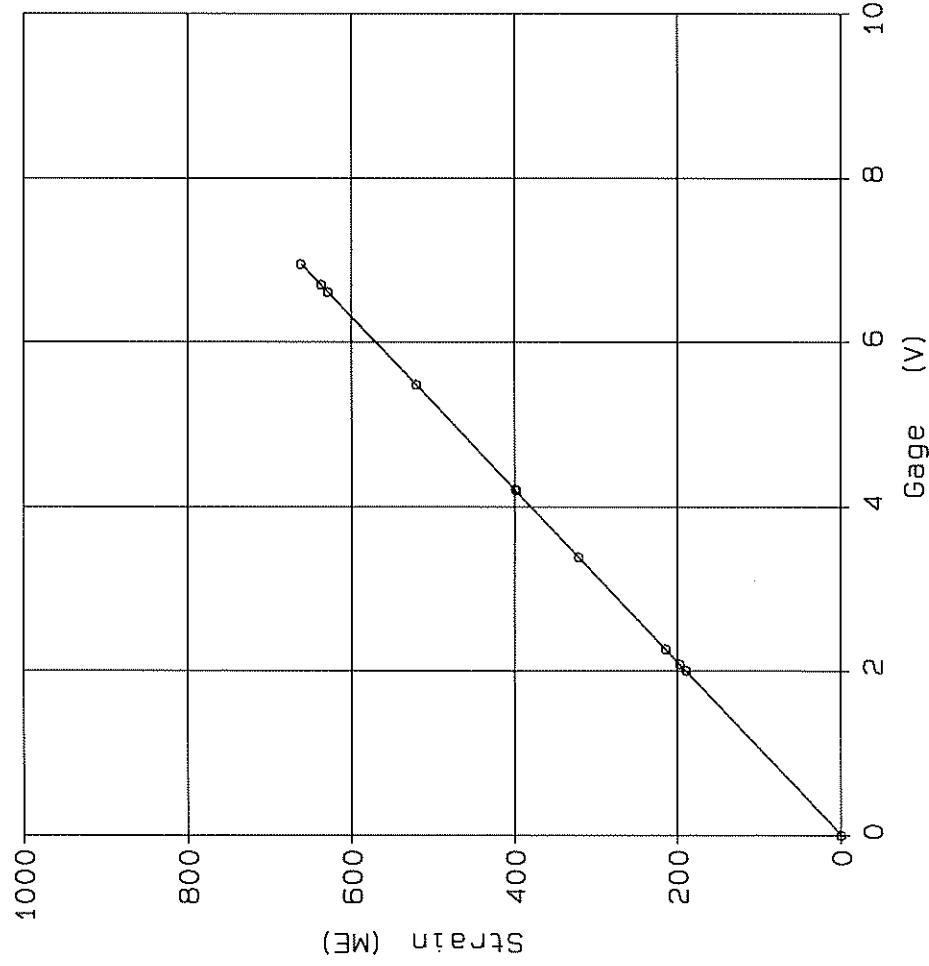

PDA Cal Factor = 95.3 ME/V
 Shunt (60.4KΩ) = 5.0 V
 General Factor = 330.8 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
189	2.00
197	2.09
214	2.27
321	3.39
400	4.21
399	4.20
521	5.48
629	6.62
637	6.70
662	6.96

Calibrated by: J. D. Dettling
 Calibrated on: 16-Jan-01