


Pile Dynamics Inc Transducer 5123

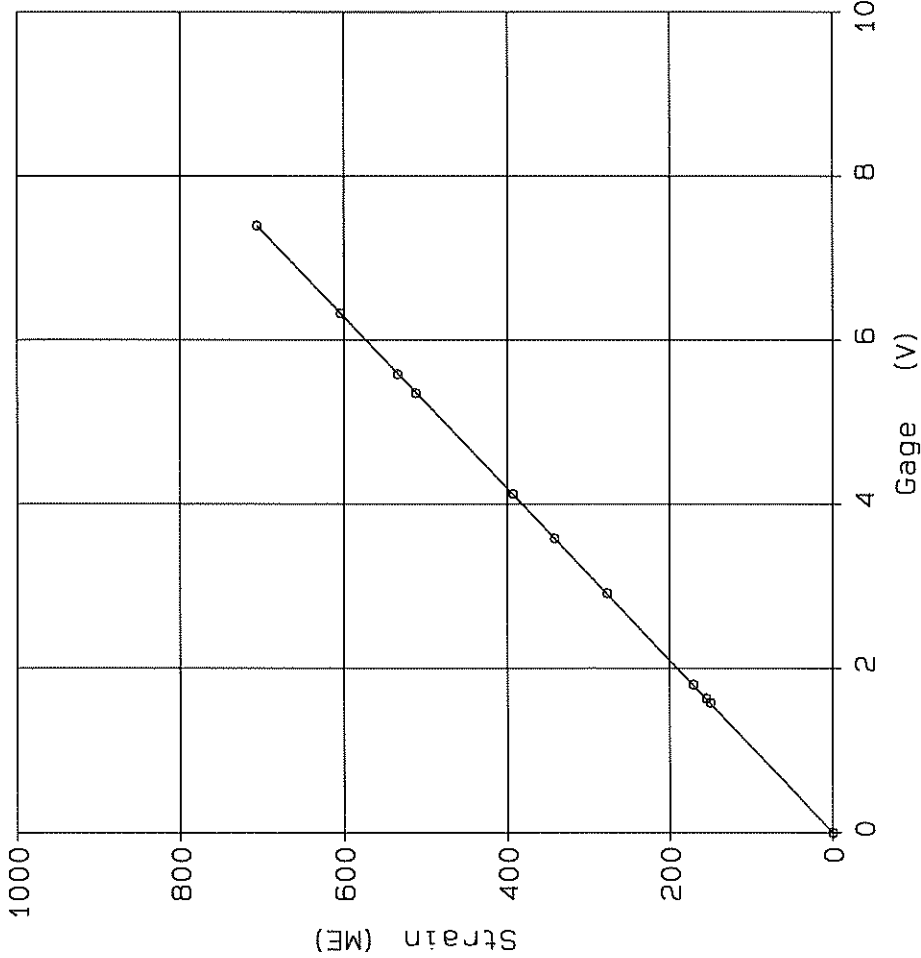

PDA Cal Factor = 95.7 ME/V
 Shunt (60.4K Ω) = 5.0 V
 General Factor = 332.1 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
151	1.59
155	1.64
172	1.81
277	2.91
342	3.59
394	4.12
512	5.12
534	5.59
604	6.32
706	7.40

Calibrated by: *J. D. Denteloff*
 Calibrated on: 16-Jan-01