


Pile Dynamics Inc Transducer 5125

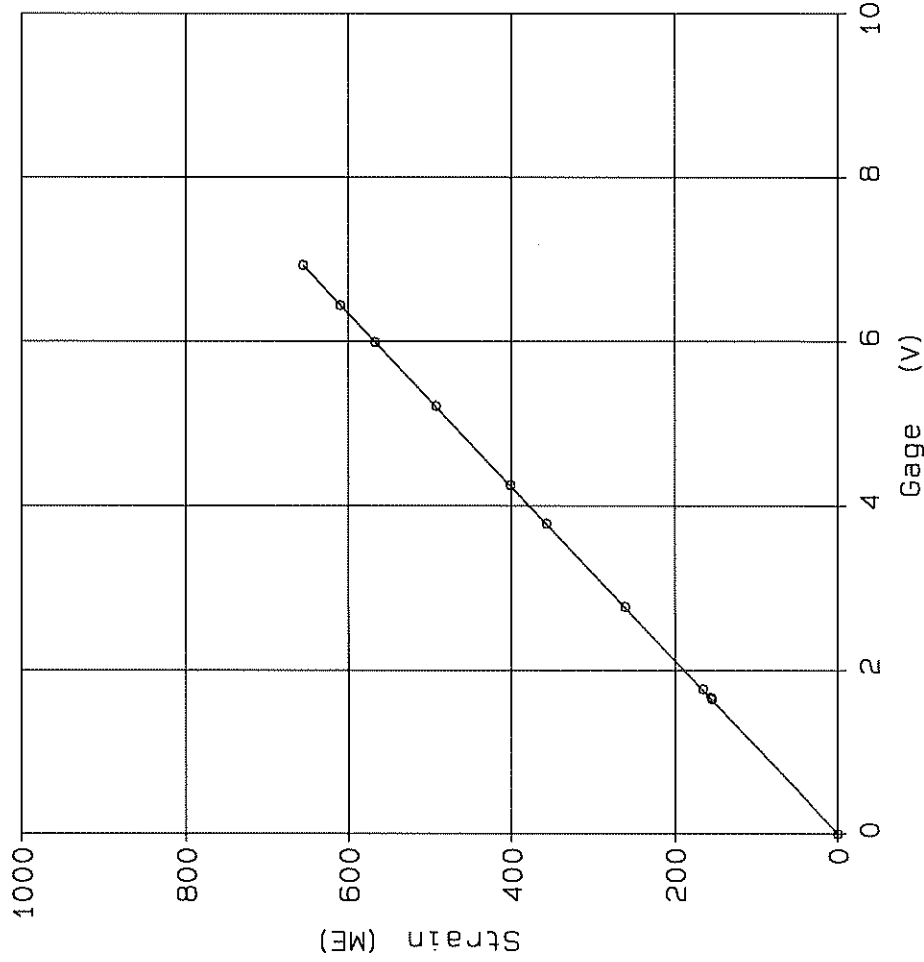

PDA Cal Factor = 94.7 ME/V
 Shunt (60.4K Ω) = 5.0 V
 General Factor = 328.9 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
157	1.67
156	1.66
167	1.77
261	2.77
357	3.78
402	4.25
493	5.21
567	5.99
610	6.45
656	6.94

Calibrated by: J. Dentley
 Calibrated on: 16-Jan-01