


Pile Dynamics Inc Transducer 5131

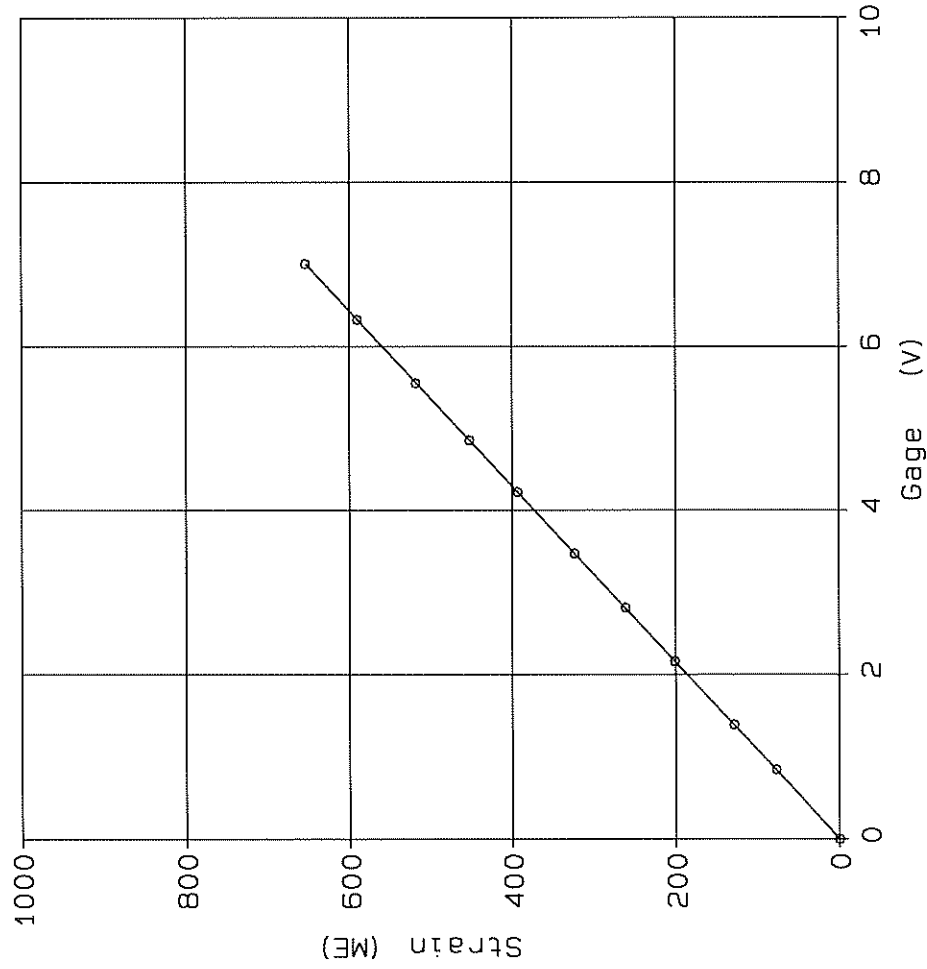

PDA Cal Factor = 93.3 ME/V
 Shunt (60.4KΩ) = 5.0 V
 General Factor = 323.9 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
79	.85
130	1.40
202	2.17
262	2.81
324	3.48
394	4.23
453	4.86
518	5.56
591	6.34
654	7.01

Calibrated by: Greg Tamba
 Calibrated on: 31-Jan-01