


Pile Dynamics Inc Transducer 5132

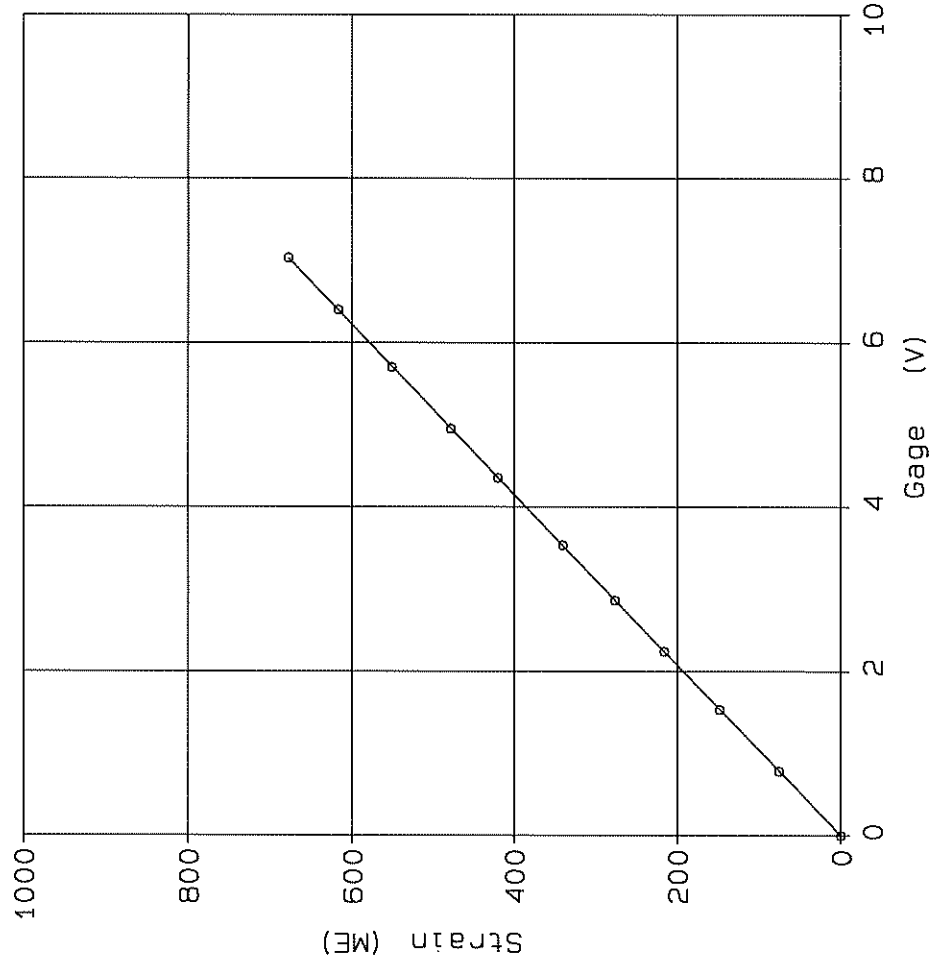

PDA Cal Factor = 96.6 ME/V
 Shunt (60.4KΩ) = 5.0 V
 General Factor = 335.2 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
76	.79
148	1.54
217	2.25
277	2.87
341	3.53
421	4.36
479	4.96
551	5.71
618	6.40
679	7.03

Calibrated by: Greg Jensen
 Calibrated on: 31-Jan-01