


Pile Dynamics Inc Transducer 5148

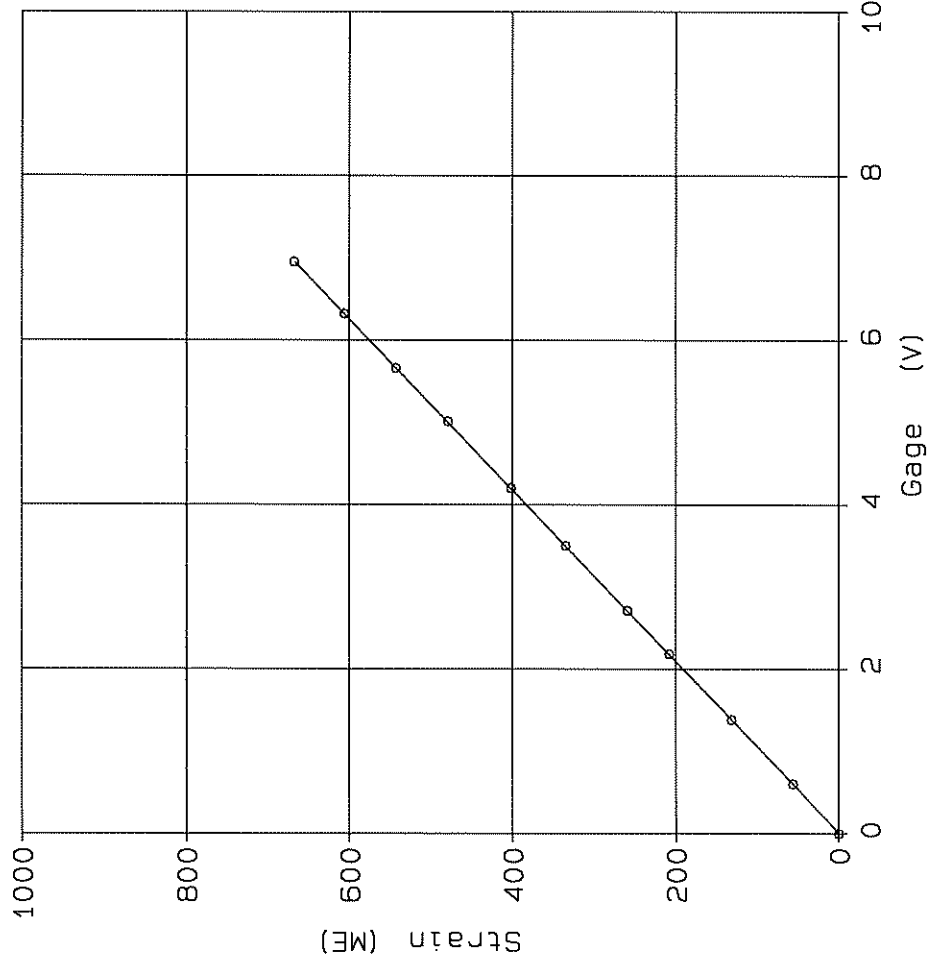

PDA Cal Factor = 96.1 ME/V
 Shunt (60.4KΩ) = 5.0 V
 General Factor = 333.6 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
57	.60
132	1.39
208	2.18
259	2.72
335	3.51
403	4.20
480	5.01
543	5.67
607	6.32
669	6.96

Calibrated by: Doug Jensen
 Calibrated on: 31-Jan-01