




Pile Dynamics, Inc.

Pile Dynamics, Inc.

Transducer 5155

Strain ($\mu\epsilon$)

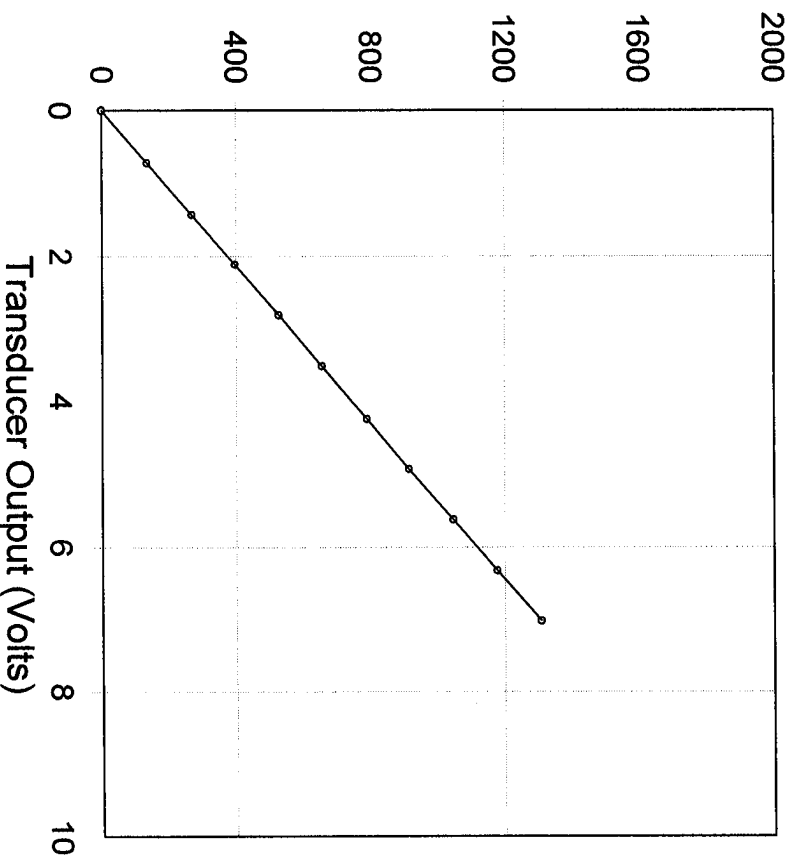

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

PDA Cal Factor (5.0 V)


92.8 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
136	0.71
268	1.42
394	2.11
524	2.81
652	3.51
787	4.24
912	4.92
1044	5.61
1176	6.32
1309	7.02

Shunt (60.4 K Ω)
General Factor

2.5 V
322.4 $\mu\epsilon/mV/V$

Calibrated by:
Calibrated on:


14-Oct-2014