



Pile Dynamics, Inc.


Pile Dynamics, Inc.

Transducer 5159

Strain ($\mu\epsilon$)

PDA Cal Factor (5.0 V)

95.7 $\mu\epsilon/V$

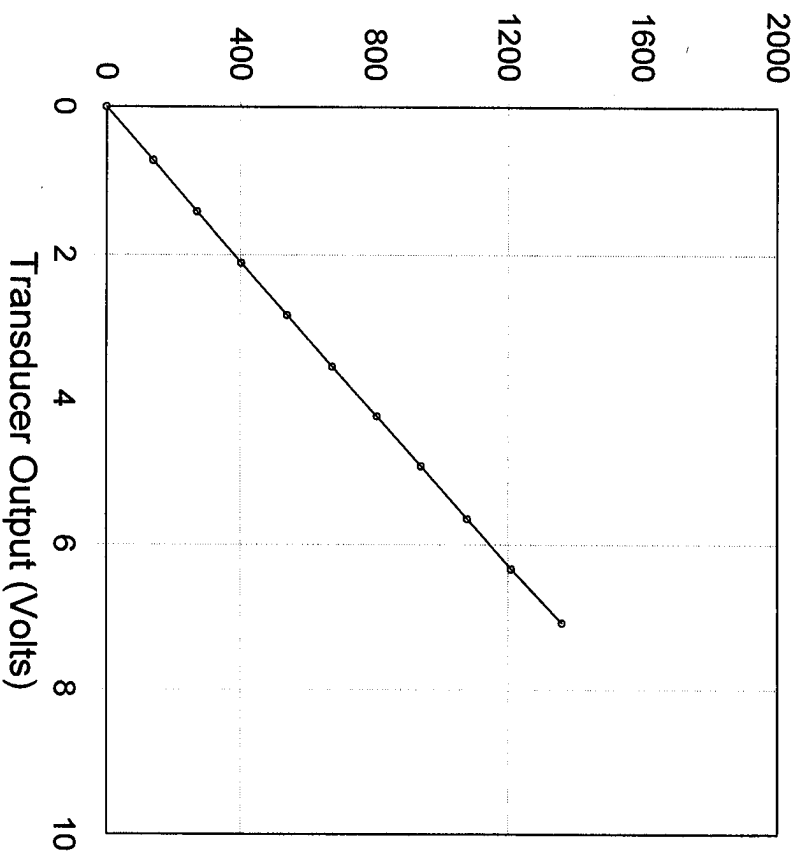

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
139	0.72
270	1.41
402	2.11
539	2.83
672	3.54
806	4.23
938	4.92
1077	5.64
1210	6.33
1359	7.07

Shunt (60.4 K Ω)

2.5 V
332.3 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by:

Calibrated on: 14-Oct-2014