


Pile Dynamics Inc Transducer 5160

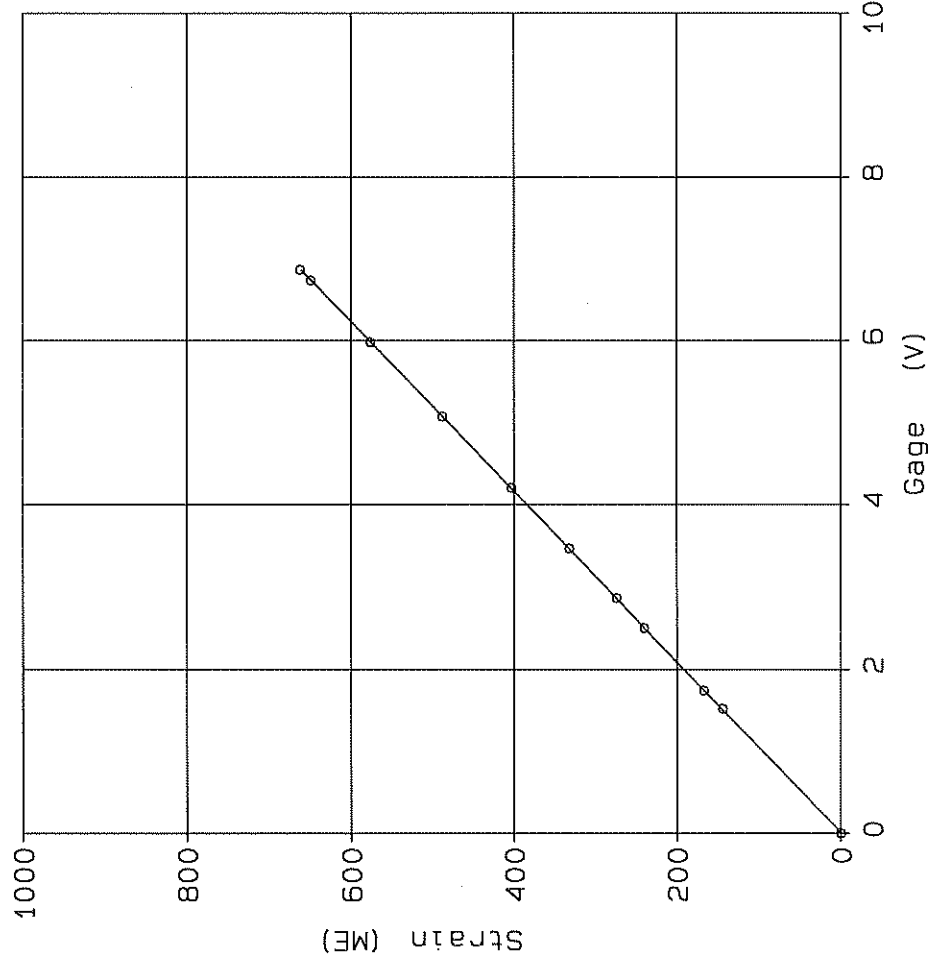

PDA Cal Factor = 96.5 ME/V
 Shunt (60.4KΩ) = 5.0 V
 General Factor = 335.0 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
145	1.52
167	1.74
241	2.51
275	2.86
333	3.46
404	4.20
489	5.08
577	5.99
650	6.74
662	6.87

Calibrated by: J. P. T. Smith

Calibrated on: 05-Jan-01