


Pile Dynamics Inc Transducer 5161

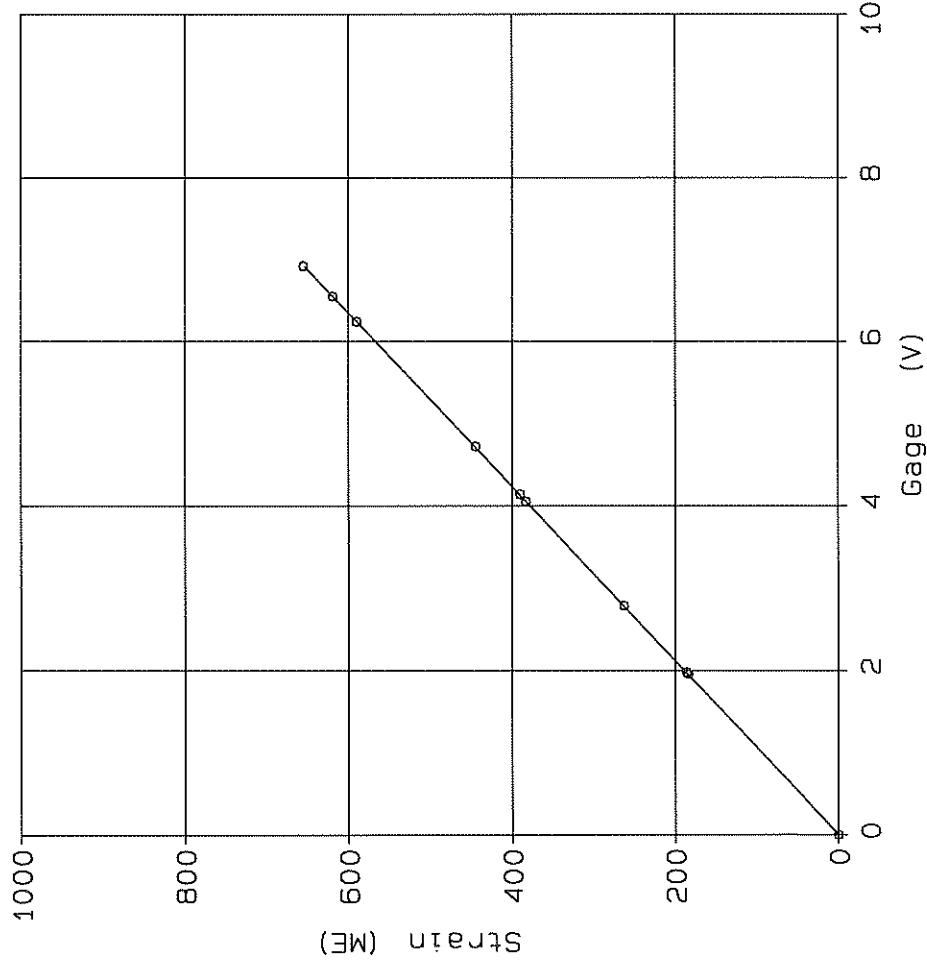

PDA Cal Factor = 94.7 ME/V
 Shunt (60.4KΩ) = 5.0 V
 General Factor = 328.7 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
187	1.98
187	1.98
185	1.96
264	2.79
383	4.05
391	4.14
446	4.72
591	6.25
619	6.55
655	6.92

Calibrated by: J. D. Dettling

Calibrated on: 05-Jan-01