


Pile Dynamics Inc Transducer 5162

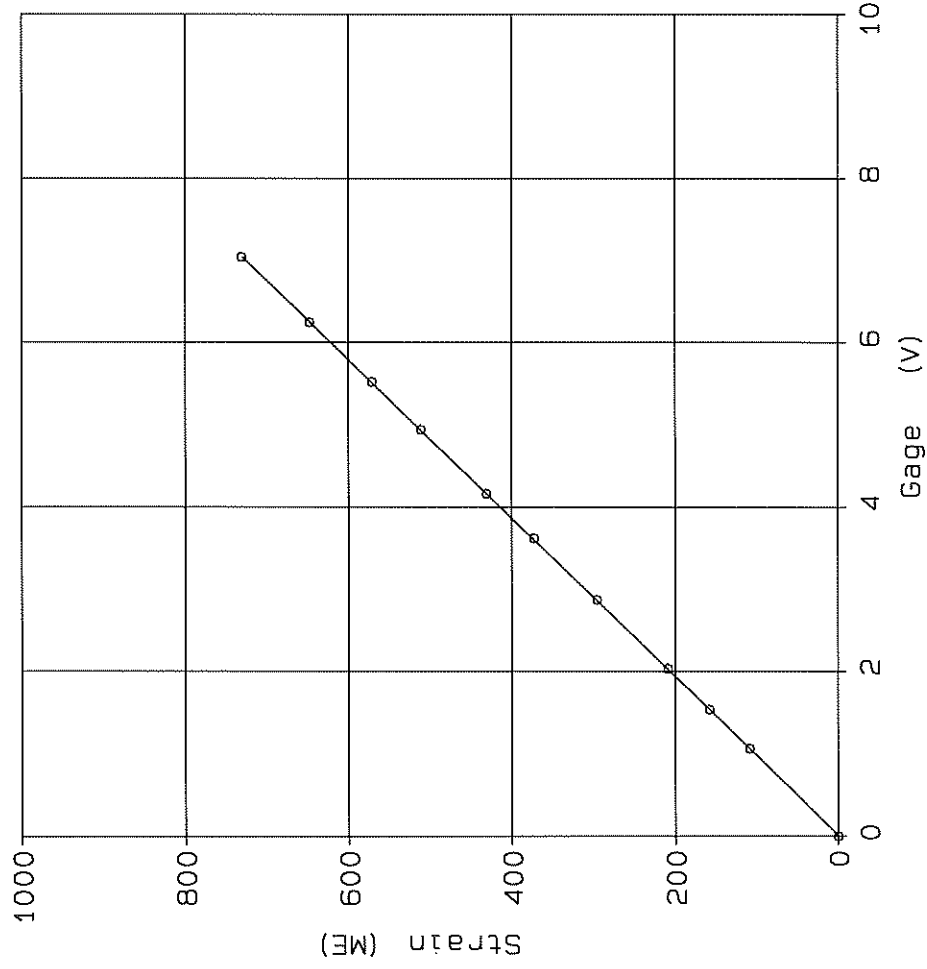

PDA Cal Factor = 103.9 ME/V
 Shunt (60.4KΩ) = 5.0 V
 General Factor = 360.9 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
110	1.06
158	1.54
210	2.03
296	2.88
374	3.62
431	4.16
512	4.94
572	5.52
649	6.24
732	7.04

Calibrated by: Reagan
 Calibrated on: 25-Jan-01