


Pile Dynamics Inc Transducer 5169

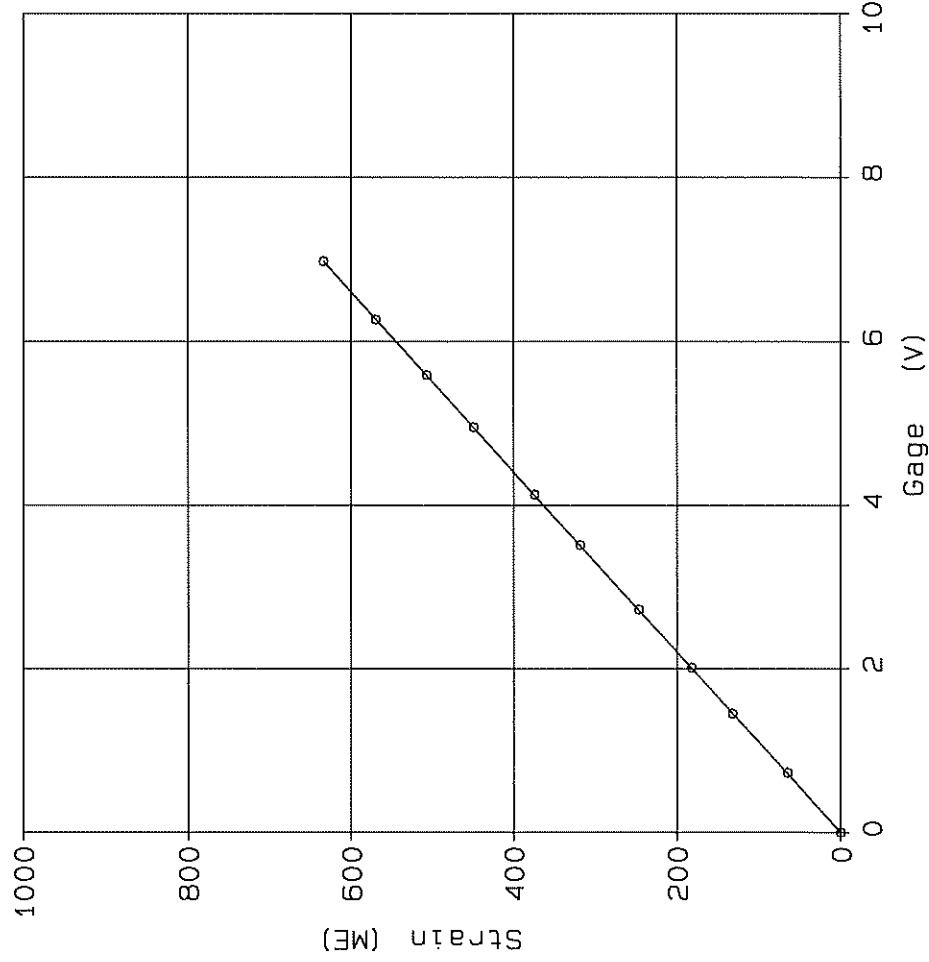

PDA Cal Factor = 90.9 ME/V
 Shunt (60.4KΩ) = 5.0 V
 General Factor = 315.5 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
66	.73
132	1.46
182	2.01
246	2.72
319	3.52
375	4.13
449	4.95
507	5.59
570	6.28
634	6.99

Calibrated by: Doug Tench

Calibrated on: 07-Feb-01