


Pile Dynamics Inc Transducer 5187

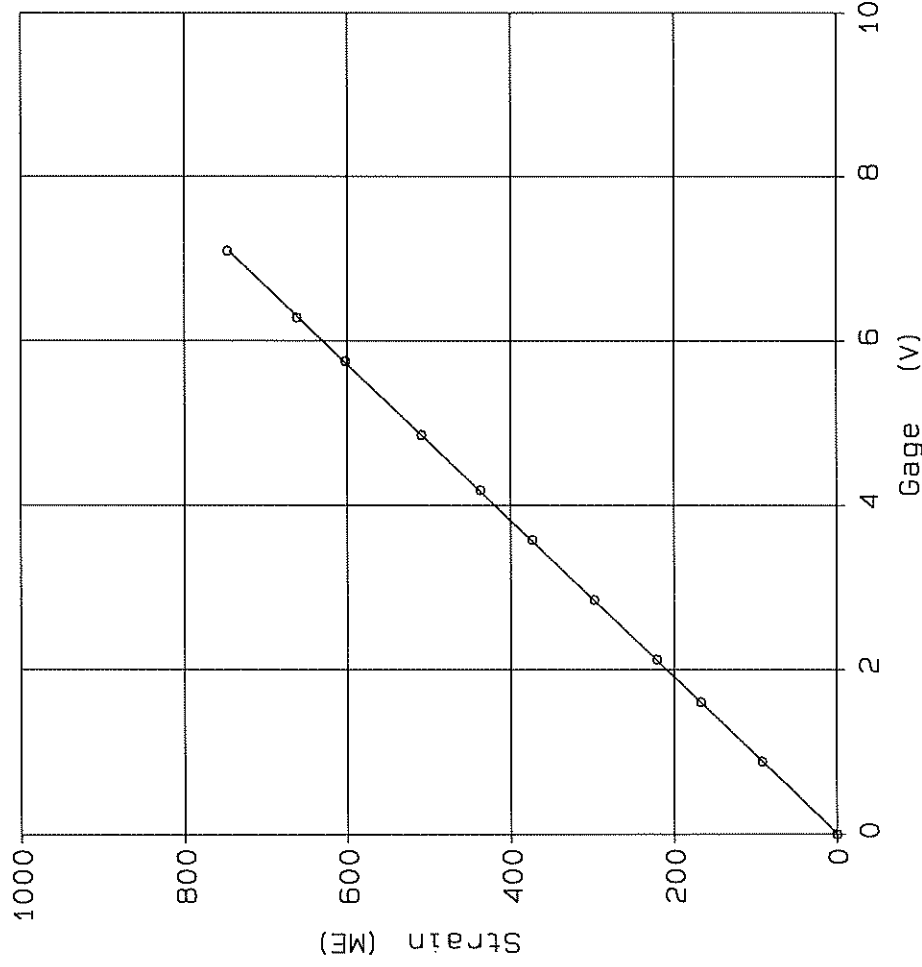

PDA Cal Factor = 105.3 ME/V
 Shunt (60.4KΩ) = 5.0 V
 General Factor = 365.7 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
93	.89
168	1.60
222	2.12
299	2.86
375	3.59
437	4.18
509	4.86
603	5.75
662	6.28
747	7.09

Calibrated by: R. Egan
 Calibrated on: 25-Jan-01