


Pile Dynamics Inc Transducer 5193

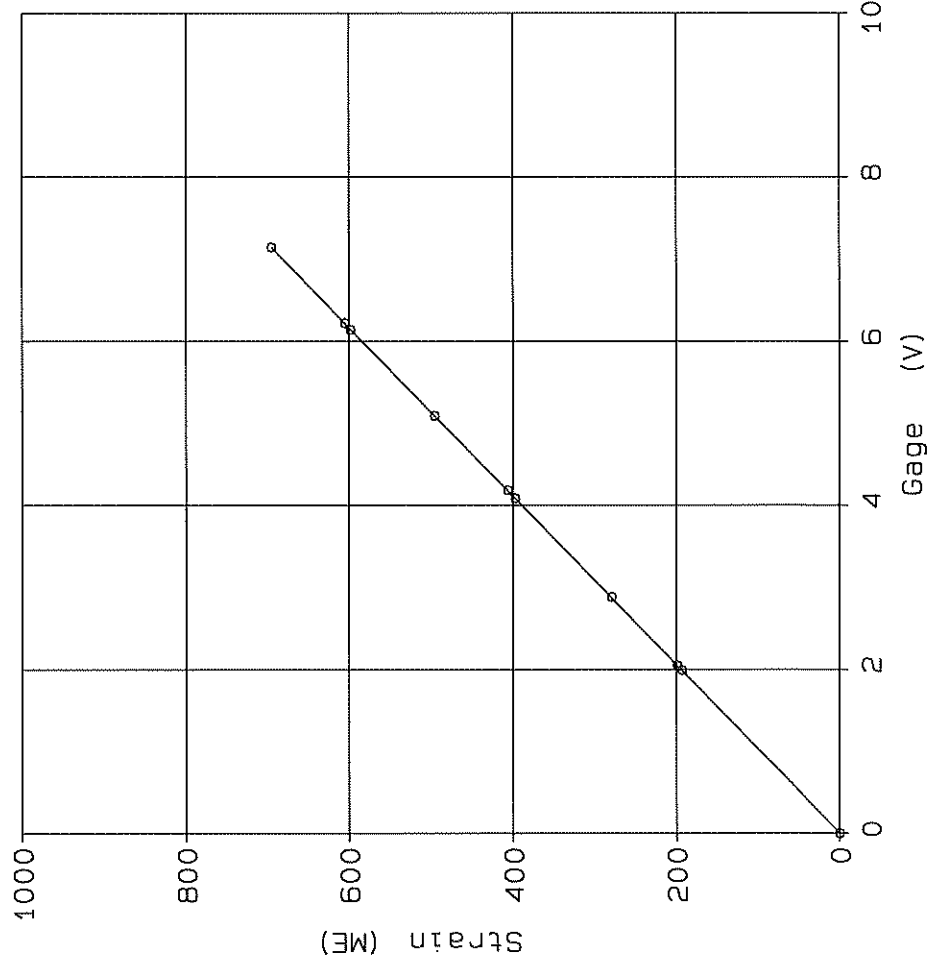

PDA Cal Factor = 97.4 ME/V
 Shunt (60.4KΩ) = 5.0 V
 General Factor = 338.2 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
194	2.00
199	2.05
199	2.05
280	2.88
398	4.09
406	4.18
495	5.09
598	6.15
606	6.23
696	7.14

Calibrated by: J. Contally
 Calibrated on: 05-Jan-01