

Certificate of Calibration

Transducer Model: PDI Transducer

Serial Number: 5197


PDI Gage Factor: 108.6 µE/V

General Gage Factor: 376.9 $~\mu\epsilon/mV/V_{ext}$ Initial Offset Voltage: 0.259 mV/V_{ext}

Table 1 – Representative Calibration Data

Applied Strain (με)	Transducer Output (mV/V _{ext})	Applied Strain (με)	Transducer Output (mV/V _{ext})
-4	0.540	271	1.279
-168	0.081	569	2.072
-455	-0.700	875	2.872
-713	-1.392	1182	3.680
-974	-2.098	1495	4.486
-1235	-2.807	1808	5.292
-1468	-3.441	2047	5.872
-1689	-4.041	2002	5.738
-1745	-4.164	1685	4.934
-1614	-3.849	1369	4.092
-1363	-3.162	1052	3.262
-1089	-2.396	741	2.442
-820	-1.655	432	1.642
-544	-0.907	135	0.862
-266	-0.149	-11	0.499
7	0.571	-11	0.511

Calibration Curve

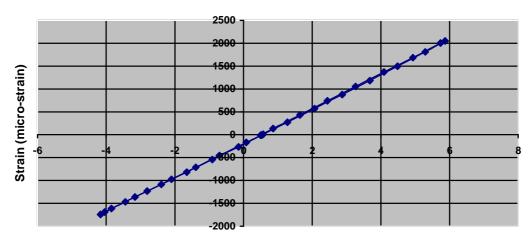

Transducer Output (mV/V)

Mean Linear Correlation Coefficient (LCC): 9.998926E-1 LCC Standard Deviation: 1.831378E-6

Calibrated By: MJ Signature:_____

Date/Time: 9/11/2015 5:53 AM Temperature (°C): 23.6

Specifications

PDI Automated Strain Transducer Calibration System (PDI-ASTCS)

ASTCS Calibration Information			
ASTCS Serial Number:	ASTCS-0005		
ASTCS Software Version:	2.310		
ASTCS Independent Verification Date:	11/5/2014 11:54 AM		
Strain Transducer Gage Length:	3.0 inches (76.2 mm)		
Applied Full Scale Displacement Range:	±7.500000E-3 inches		
Method for Applying Displacement:	Precision Step Motor Coupled to Linear Stage		
Excitation Voltage for Calibration:	2.5 VDC		
Displacement Measurements:	Dual Precision AC LVDT's, Output Averaged		
Displacement Certification:	NIST 274437-07		
Linearity Verification Technique:	Linear Correlation Coefficient > 0.9999		
Repeatability Verification Technique:	Standard Deviation < 0.5 % (of mean)		
ASTCS System Check			
Reference Strain Transducer:	4367T		
Reference General Gage Factor:	293.000 με/mV/V		
LVDT #1 Sensitivity (inches/volt):	7.916500E-3		
LVDT #2 Sensitivity (inches/volt):	8.042000E-3		
Date/Time of Last System Check:	9/11/2015 5:40 AM		
PDI Strain Transducer Connections			
Black:	+ Excitation		
Green:	- Excitation		
Red:	+ Signal		
White:	- Signal		
Grey:/BARE	Shield		

NIST Reference:

PDI certifies the above PDI-ASTCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique. The calibration of this instrument was performed in accordance with the PDI Quality Assurance program. Measurements and information provided on this report are valid at the time of calibration only.