


Pile Dynamics Inc Transducer 5198

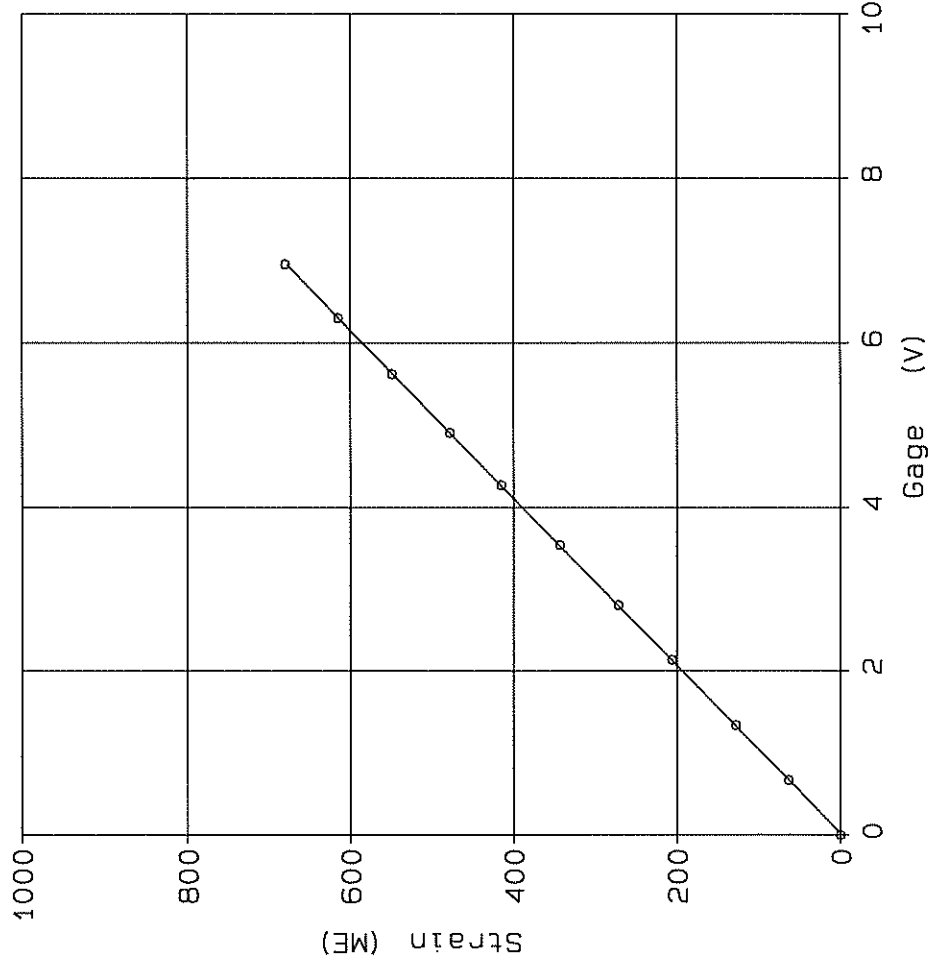

PDA Cal Factor = 97.9 ME/V
 Shunt (60.4KΩ) = 5.0 V
 General Factor = 339.8 ME/mV/V
 Traceable to N.I.S.T.

Strain ME	Gage V
0	.00
64	.67
128	1.34
206	2.14
272	2.81
343	3.54
415	4.27
479	4.92
549	5.63
615	6.30
680	6.96

Calibrated by: J. J. Cantrell
 Calibrated on: 28-Jan-03