




Pile Dynamics, Inc.

Transducer A177

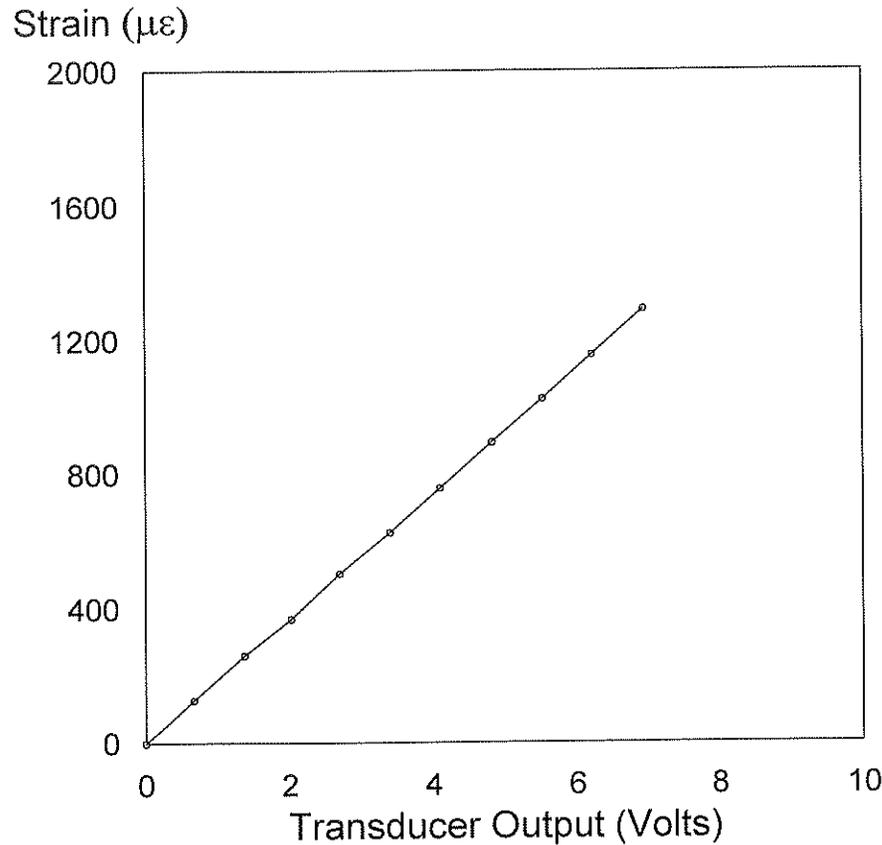

PDA Cal Factor (5.0 V) 92.8με/V

Applied Strain (με)	Transducer Output (Volts)
0	0.00
128	0.66
260	1.37
370	2.02
502	2.70
625	3.40
756	4.10
893	4.81
1023	5.52
1155	6.20
1292	6.94

Shunt (60.4 KΩ) 2.5 V
 General Factor 322.2με/mV/V

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Calibrated by: 
 Calibrated on: 19-Aug-2011