




Pile Dynamics, Inc.

Pile Dynamics, Inc.

Transducer A182

Strain ($\mu\epsilon$)

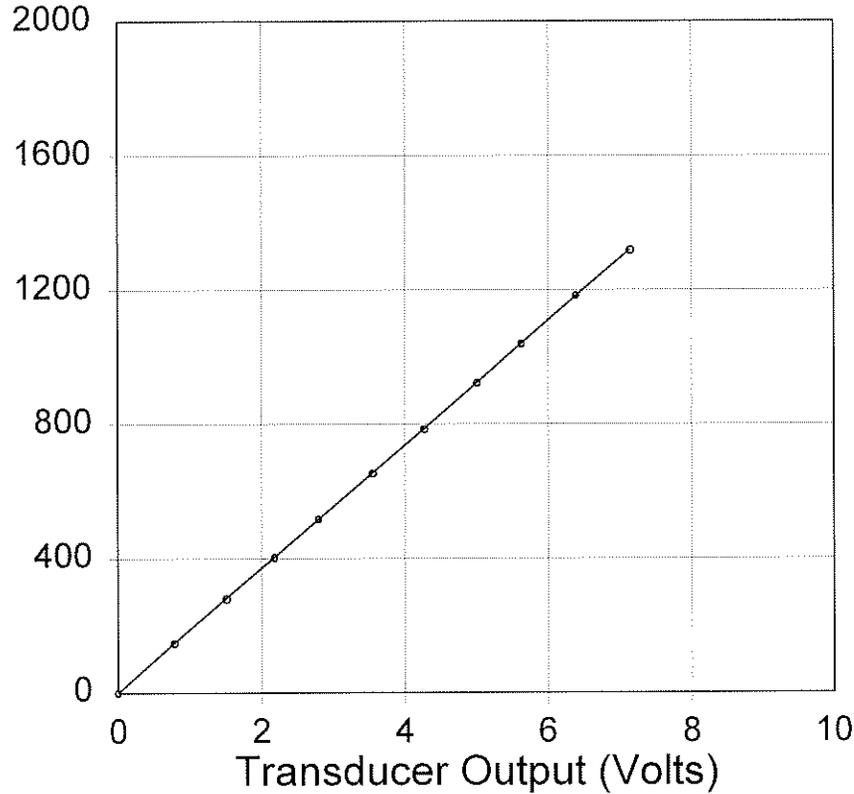

PDA Cal Factor (5.0 V) 92.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
149	0.78
281	1.50
403	2.18
517	2.79
654	3.54
786	4.26
923	5.00
1041	5.63
1182	6.40
1319	7.14

Shunt (60.4 K Ω) 2.5 V
General Factor 319.8 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by: Fred Hein
Calibrated on: 02-Jun-2006