



Certificate of Calibration

Pile Dynamics, Inc.

Transducer Model: PDI Strain Transducer

Serial Number: B642


PDI Gage Factor: 91.3

Mean Linear Correlation Coefficient: 0.999766

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2021.0	-6.216	380.6	1.566
-1627.3	-4.924	820.2	2.905
-1292.7	-3.776	1148.3	3.966
-925.2	-2.573	1496.1	5.023
-518.4	-1.267	1837.3	6.056
-59.1	0.169	1983.8	6.482

Calibration Curve

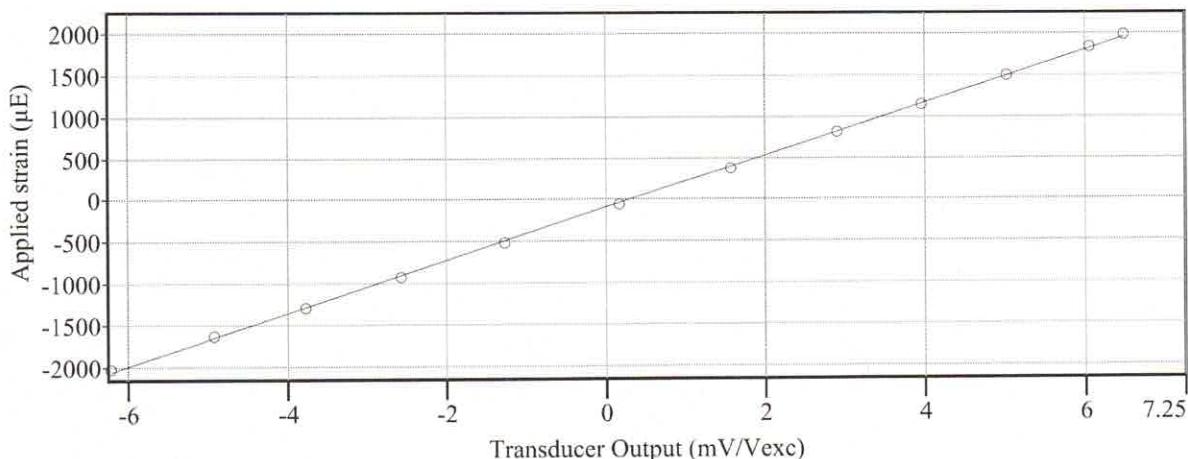

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: Paul Hartman

PDI Gage: B642

Calibration Date: 4/13/2023 4:43:23 AM

