




Pile Dynamics, Inc.

Transducer B644

Strain ($\mu\epsilon$)

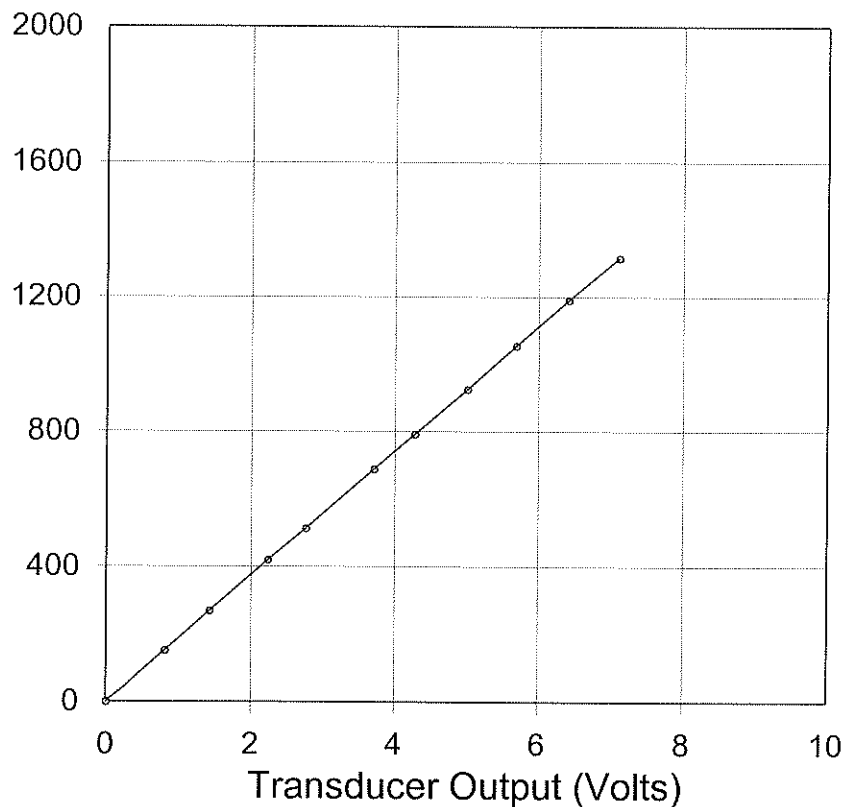

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

PDA Cal Factor (5.0 V)

92.5 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
152	0.80
270	1.42
418	2.24
512	2.76
688	3.70
792	4.27
926	5.00
1055	5.68
1191	6.42
1318	7.11

Shunt (60.4 K Ω)

2.5 V

General Factor

321.1 $\mu\epsilon$ /mV/V

Calibrated by:

Stacy

Calibrated on:

20-Jul-2007