




Pile Dynamics, Inc.

Transducer B648

Strain ($\mu\epsilon$)

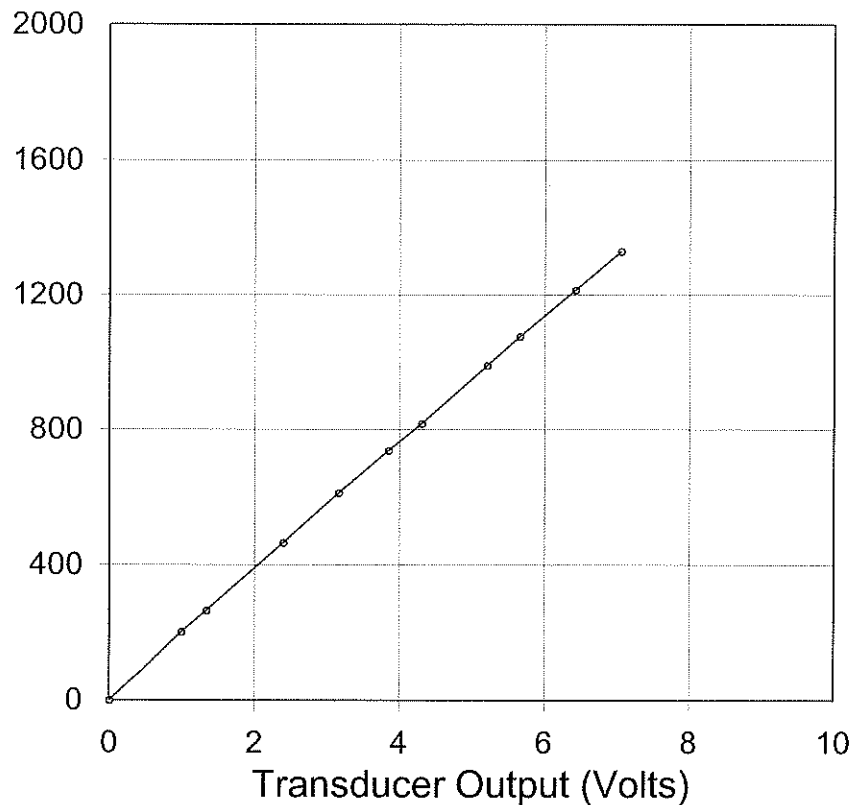

PDA Cal Factor (5.0 V)

93.8 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
203	0.98
266	1.32
464	2.39
612	3.15
737	3.85
818	4.30
991	5.20
1077	5.65
1215	6.42
1331	7.05

Shunt (60.4 K Ω)

2.5 V

General Factor

325.8 $\mu\epsilon$ /mV/V

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by:

George Pinnell

Calibrated on:

18-Jul-2007