




Pile Dynamics, Inc.

Transducer B650

Strain ($\mu\epsilon$)

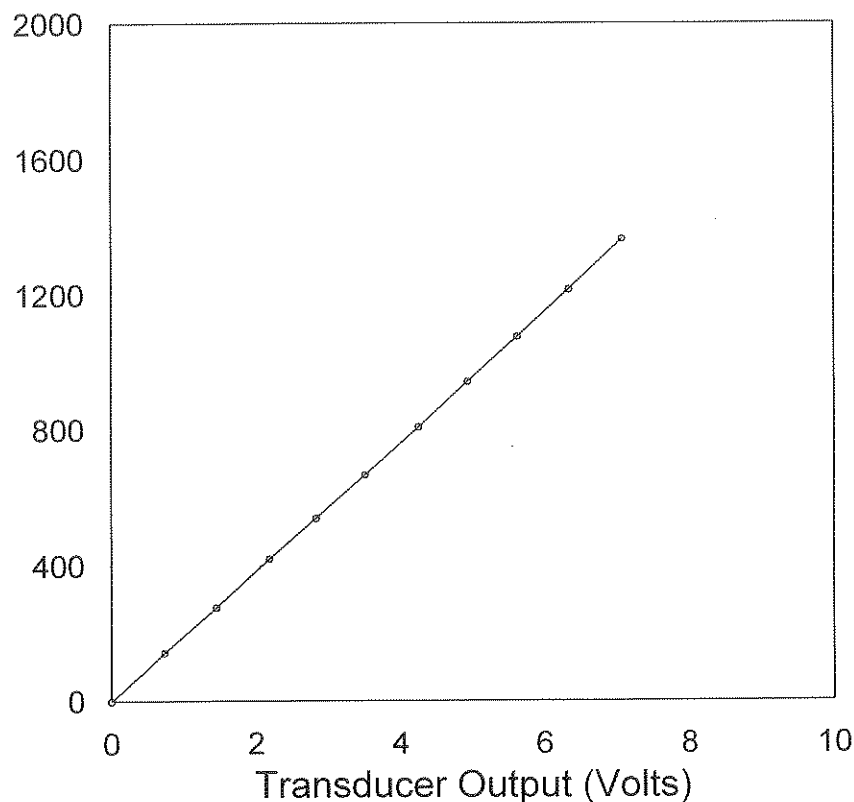

PDA Cal Factor (5.0 V)

95.9 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
144	0.73
276	1.44
419	2.19
537	2.83
665	3.51
807	4.25
940	4.93
1075	5.62
1215	6.33
1365	7.07

Shunt (60.4 K Ω)

2.5 V

General Factor

333.1 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by: *Eric S. Smith*
 Calibrated on: 12-Sep-2013

Smart Sensor? ☒ Yes ☐ No Smart Chip Programmed by: E.S. Date: 9-12-13 CRC value 727E