




Pile Dynamics, Inc.

Transducer B654

Strain ($\mu\epsilon$)

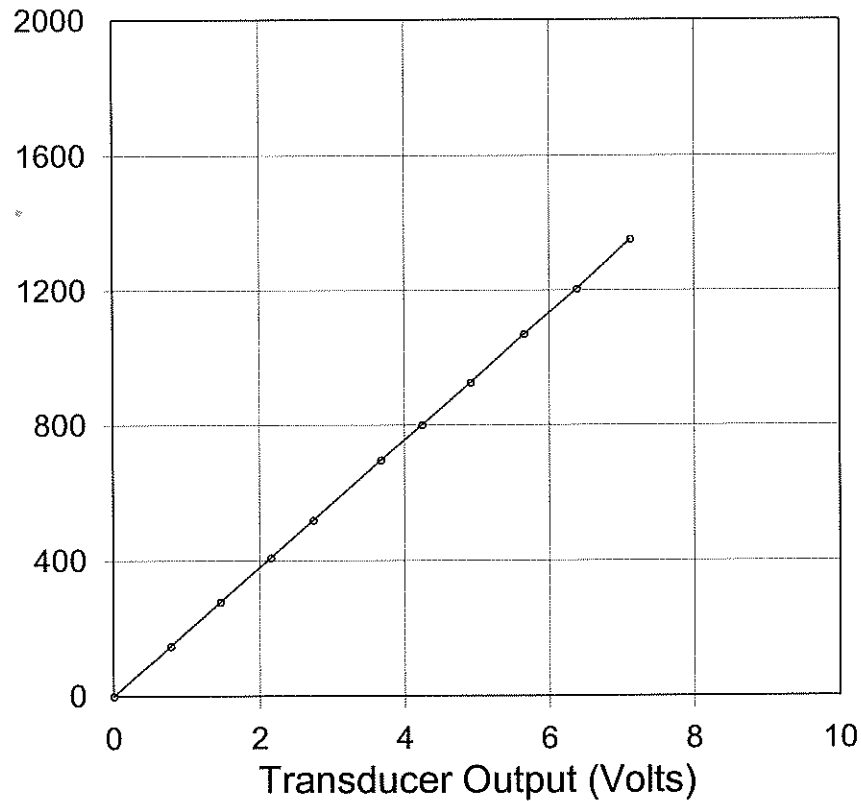

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

PDA Cal Factor (5.0 V)

94.5 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
149	0.77
278	1.45
409	2.15
519	2.73
696	3.67
799	4.24
925	4.91
1070	5.65
1206	6.38
1352	7.12

Shunt (60.4 K Ω)

2.5 V

General Factor

328.0 $\mu\epsilon$ /mV/V

Calibrated by:

Shaul

Calibrated on:

02-Oct-2007