




Pile Dynamics, Inc.

Transducer B978

Strain ($\mu\epsilon$)

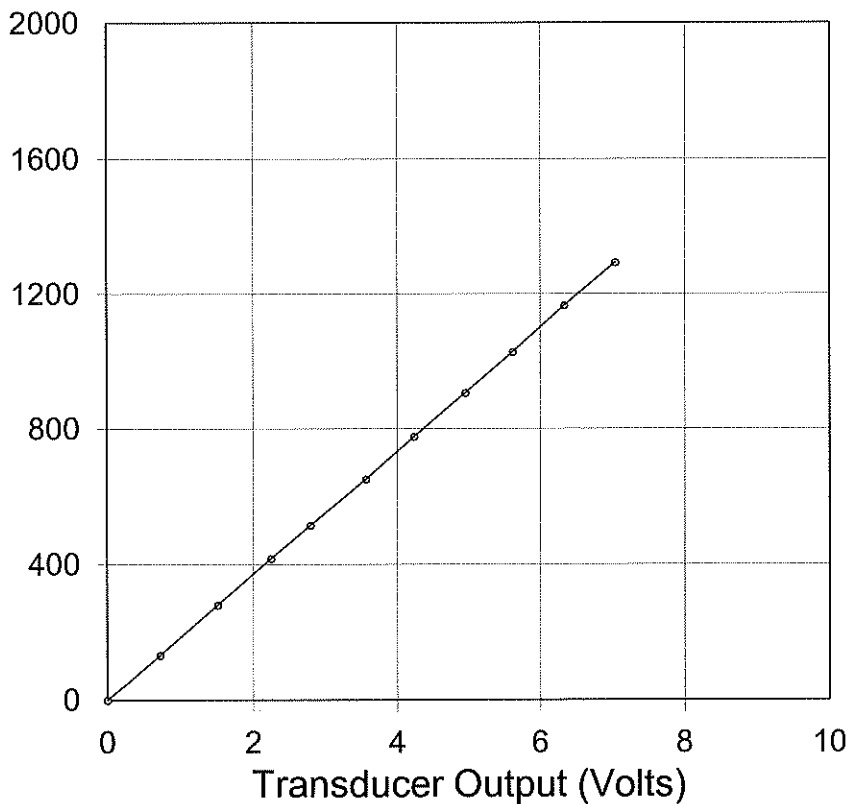

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

PDA Cal Factor (5.0 V)

91.6 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
133	0.70
279	1.50
417	2.25
515	2.79
650	3.56
776	4.23
907	4.95
1028	5.61
1165	6.33
1294	7.04

Shunt (60.4 K Ω)
General Factor

2.5 V
318.2 $\mu\epsilon$ /mV/V

Calibrated by:

Calibrated on:

Shah
04-Dec-2007