




Pile Dynamics, Inc.

Transducer B979

Strain ($\mu\epsilon$)

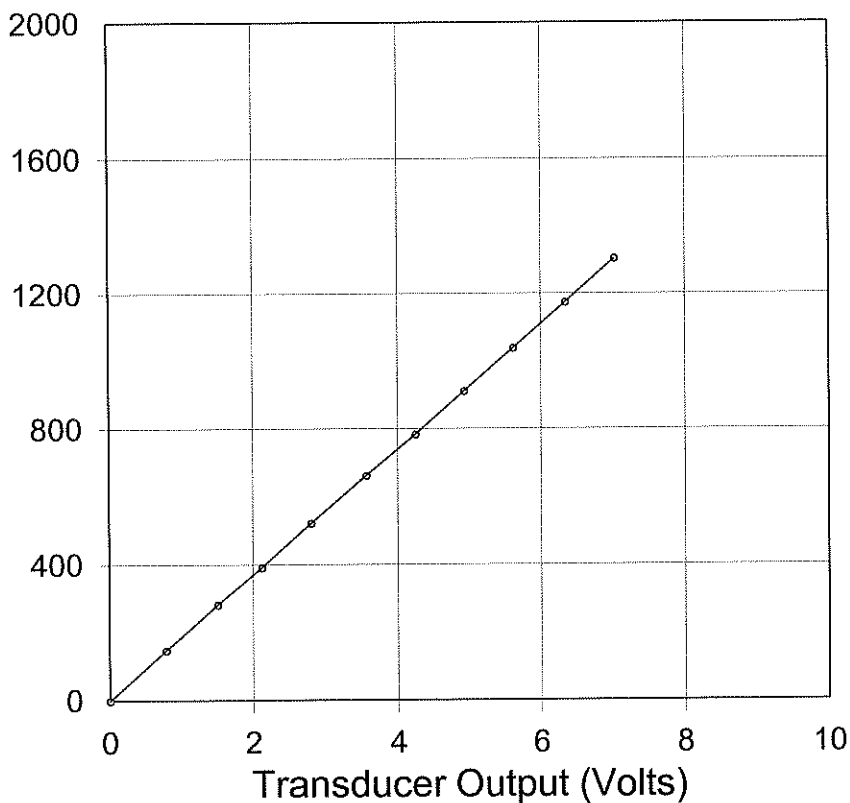

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

PDA Cal Factor (5.0 V)

92.5 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
149	0.78
282	1.50
392	2.12
520	2.80
662	3.56
783	4.24
911	4.92
1037	5.61
1175	6.34
1305	7.03

Shunt (60.4 K Ω)

2.5 V

General Factor

321.2 $\mu\epsilon$ /mV/V

Calibrated by:

Shael

Calibrated on:

04-Dec-2007