




Pile Dynamics, Inc.

Transducer B980

Strain ($\mu\epsilon$)

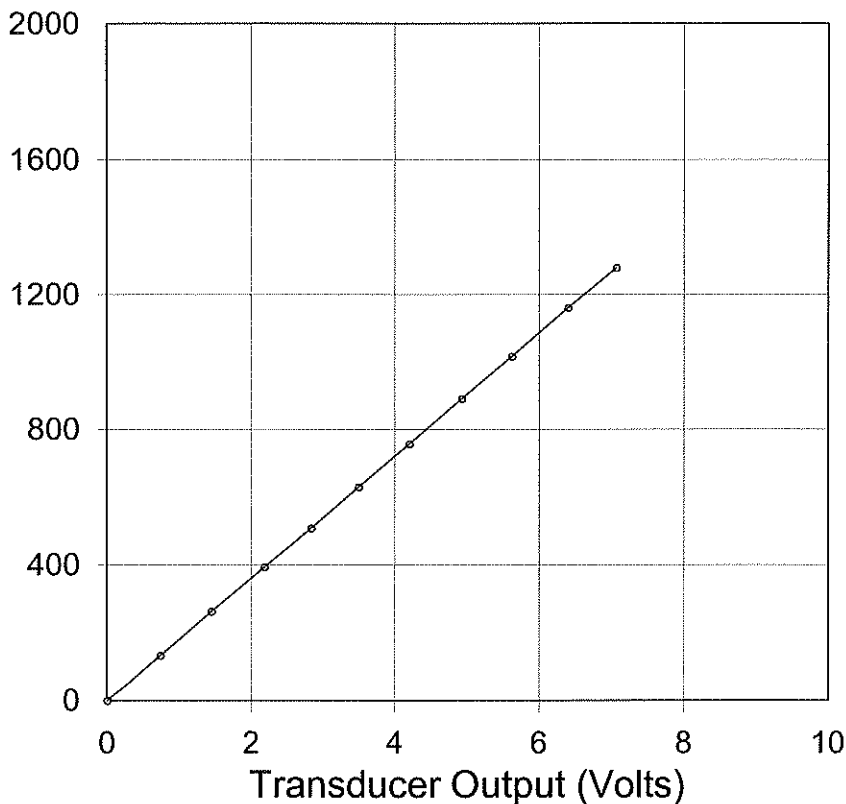

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

PDA Cal Factor (5.0 V)

90.6 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
133	0.73
263	1.44
394	2.18
508	2.83
630	3.49
756	4.20
891	4.93
1017	5.62
1161	6.39
1280	7.06

Shunt (60.4 K Ω)
General Factor

2.5 V

314.4 $\mu\epsilon$ /mV/V

Calibrated by:

Calibrated on:

04-Dec-2007